

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-100101_P1-B-1_01_9567.d
 Method lc ms directos_241016neg.m
 Sample Name 24-100101
 Comment JM-01
 Sv: DCM + MeOH + HCOOH
 Argüello - UNC

Acquisition Date 10/16/2024 12:14:49 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

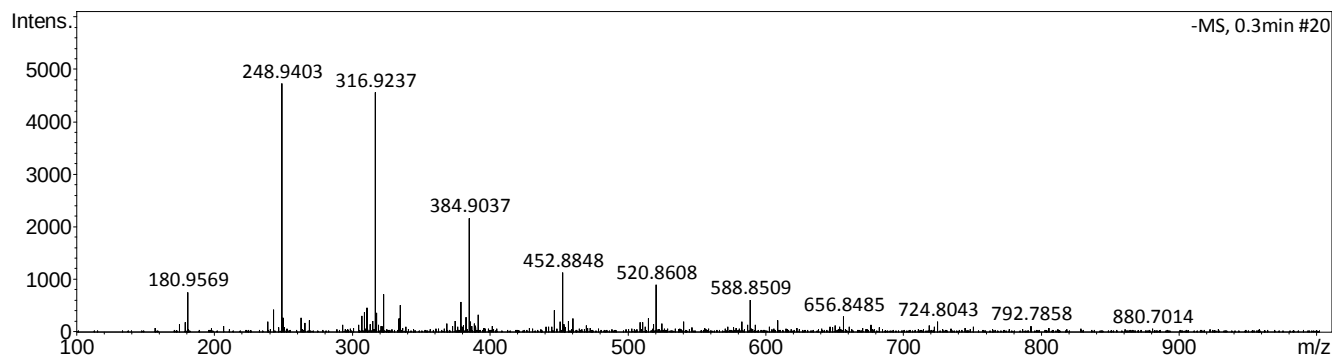

#	m/z	I	I %
1	180.9569	749	15.9
2	242.9225	424	9.0
3	248.9403	4715	100.0
4	249.9429	268	5.7
5	263.0642	261	5.5
6	268.9604	219	4.6
7	306.8978	302	6.4
8	309.0639	381	8.1
9	310.9031	457	9.7
10	314.9026	211	4.5
11	316.9237	4554	96.6
12	317.9216	367	7.8
13	322.9201	695	14.7
14	322.9549	641	13.6
15	323.0070	710	15.1
16	333.9076	254	5.4
17	334.9436	504	10.7
18	378.8868	565	12.0
19	382.8829	279	5.9
20	384.9037	2161	45.8
21	391.5672	324	6.9
22	446.8699	407	8.6
23	452.8848	1125	23.9
24	456.8575	212	4.5
25	460.1805	253	5.4
26	514.8468	254	5.4
27	520.8608	903	19.2
28	588.8509	611	13.0
29	608.7906	220	4.7
30	656.8485	295	6.3