

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-100102_P1-B-2_01_9568.d
 Method lc ms directos_241016neg.m
 Sample Name 24-100102
 Comment JM-02
 Sv: DCM + MeOH + HCOOH
 Argüello - UNC

Acquisition Date 10/16/2024 12:19:57 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

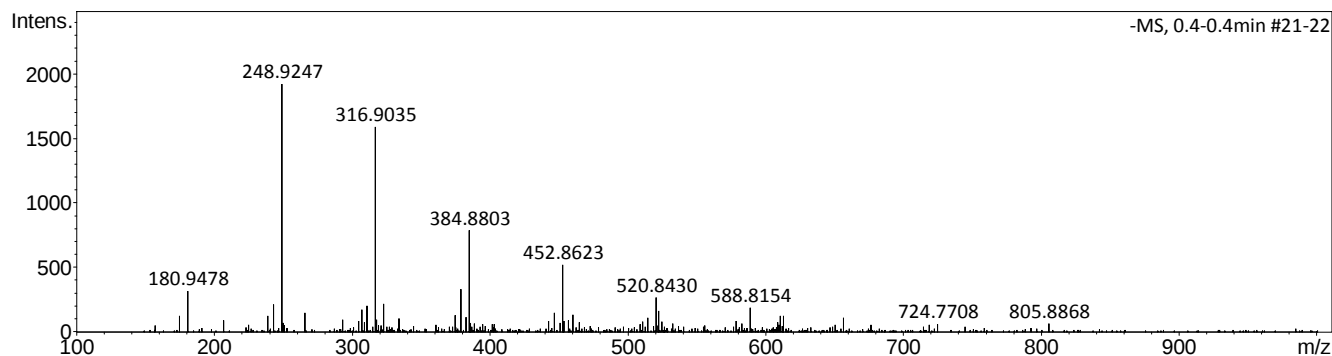

#	m/z	I	I %
1	174.9333	122	6.4
2	180.9478	316	16.5
3	206.9442	89	4.6
4	238.8958	122	6.3
5	242.9078	211	11.0
6	248.9247	1919	100.0
7	265.9155	148	7.7
8	292.9414	95	4.9
9	304.8685	86	4.5
10	306.8757	175	9.1
11	310.8889	202	10.5
12	316.9035	1586	82.6
13	317.9062	96	5.0
14	322.9463	218	11.4
15	333.8849	105	5.5
16	374.8518	127	6.6
17	378.8635	329	17.1
18	382.8407	112	5.8
19	384.8803	787	41.0
20	446.8395	149	7.8
21	452.8623	520	27.1
22	456.8351	88	4.6
23	460.1080	132	6.9
24	514.8154	110	5.7
25	520.8430	268	14.0
26	522.4572	162	8.4
27	588.8154	186	9.7
28	610.9186	124	6.4
29	612.9117	124	6.5
30	656.7938	110	5.7