

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\24-100104_P1-B-4_01_9570.d
 Method lc ms directos_241016neg.m
 Sample Name 24-100104
 Comment JM-04
 Sv: DCM + MeOH + HCOOH
 Argüello - UNC

Acquisition Date 10/16/2024 12:31:35 PM

Operator EB - MV
 Instrument / Ser# microTOF-Q

Acquisition Parameter

Source Type	ESI	Ion Polarity	Negative	Set Nebulizer	2.0 Bar
Focus	Not active	Set Capillary	3500 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	250.0 Vpp	Set Divert Valve	Source

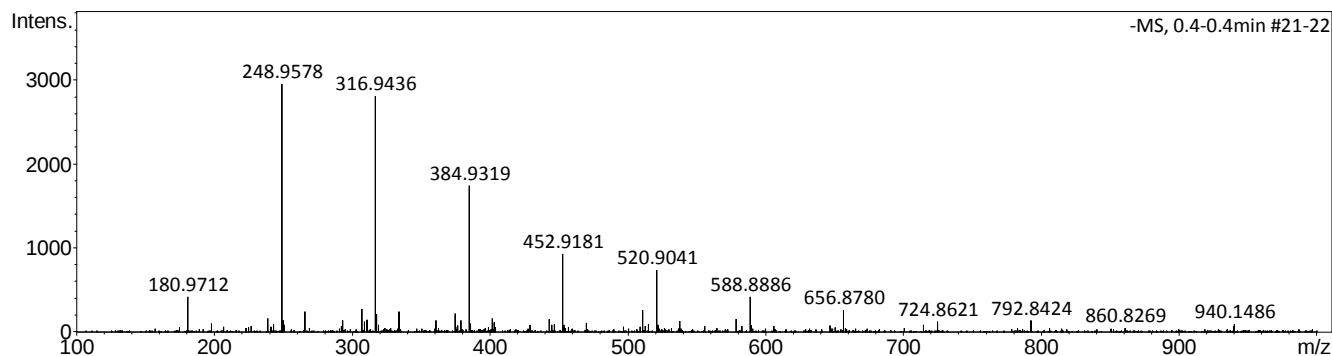

#	m/z	I	I %
1	180.9712	415	14.1
2	197.9627	101	3.4
3	238.9262	159	5.4
4	248.9578	2945	100.0
5	249.9626	139	4.7
6	265.9474	242	8.2
7	292.9879	136	4.6
8	306.9150	275	9.3
9	308.9120	122	4.1
10	310.9302	142	4.8
11	316.9436	2802	95.1
12	317.9478	214	7.3
13	333.9368	246	8.3
14	360.9675	137	4.6
15	374.9039	223	7.6
16	378.9094	139	4.7
17	384.9319	1737	59.0
18	401.9218	156	5.3
19	403.3027	115	3.9
20	442.8910	153	5.2
21	452.9181	925	31.4
22	469.9112	109	3.7
23	510.8735	261	8.9
24	520.9041	734	24.9
25	537.8949	128	4.3
26	578.8634	155	5.3
27	588.8886	419	14.2
28	656.8780	258	8.7
29	724.8621	123	4.2
30	792.8424	136	4.6