

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\Eve\US-44 despues de calentar con HCOOH.d
Method Tune_low_formate 210120.m
Sample Name US-44 despues de calentar
Comment Agregado de HCOOH
Cecilia

Acquisition Date 8/25/2022 3:20:19 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	950 m/z	Set Collision Cell RF	150.0 Vpp	Set Divert Valve	Source

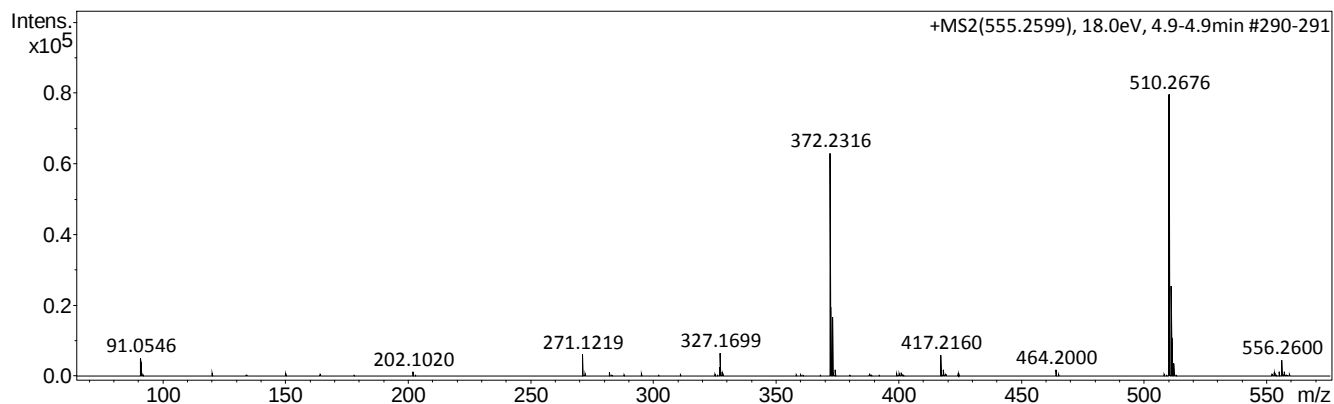

#	m/z	I	I %
1	91.0546	5072	6.4
2	120.0814	910	1.1
3	150.0351	763	1.0
4	202.1020	1278	1.6
5	271.1219	6192	7.8
6	272.1236	779	1.0
7	282.1833	1137	1.4
8	295.1794	892	1.1
9	325.1875	683	0.9
10	327.1699	6573	8.3
11	328.1724	947	1.2
12	372.2316	62809	79.1
13	373.2345	16723	21.1
14	374.2367	1946	2.5
15	399.2178	754	0.9
16	400.2246	829	1.0
17	401.2208	715	0.9
18	417.2160	6096	7.7
19	418.2198	1874	2.4
20	424.4928	875	1.1
21	464.2000	1941	2.4
22	465.1973	699	0.9
23	508.2531	565	0.7
24	510.2676	79417	100.0
25	511.2719	25491	32.1
26	512.2738	3735	4.7
27	553.2922	1013	1.3
28	555.2599	1318	1.7
29	556.2600	4564	5.7
30	557.2631	1300	1.6