

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\Eve\US-44 despues de calentar.d
Method Tune_low_formate 210120.m
Sample Name US-44 despues de calentar
Comment Cecilia

Acquisition Date 8/25/2022 3:06:30 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	950 m/z	Set Collision Cell RF	150.0 Vpp	Set Divert Valve	Source

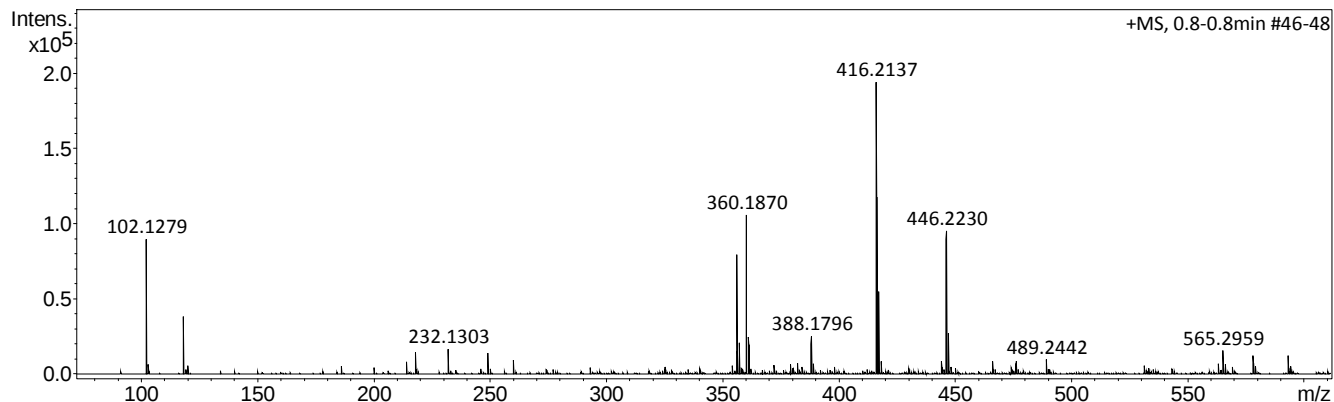

#	m/z	I	I %
1	102.1279	89545	46.2
2	103.1304	6519	3.4
3	118.1221	38077	19.7
4	214.1410	8127	4.2
5	218.1150	14484	7.5
6	232.1303	16421	8.5
7	249.1378	14087	7.3
8	260.1256	9605	5.0
9	356.2125	79359	41.0
10	357.2157	20691	10.7
11	360.1870	105610	54.5
12	361.1907	24833	12.8
13	379.1959	6380	3.3
14	382.1732	7204	3.7
15	388.1796	25134	13.0
16	389.1844	6727	3.5
17	416.2137	193754	100.0
18	417.2165	54637	28.2
19	418.2149	8644	4.5
20	444.2612	8674	4.5
21	446.2230	95165	49.1
22	447.2268	27096	14.0
23	466.2445	8690	4.5
24	476.2330	8765	4.5
25	489.2442	9743	5.0
26	563.2777	6726	3.5
27	565.2959	15774	8.1
28	566.2966	6418	3.3
29	578.2425	12266	6.3
30	593.3256	12293	6.3