

Qualitative Compound Report

Analysis Info

Analysis Name D:\Data\Eve\US-44 con HCOOH.d
Method Tune_low_format 210120.m
Sample Name US-44
Comment Agregado de HCOOH
Cecilia


Acquisition Date 8/26/2022 10:27:38 AM

Operator ELB
Instrument micrOTOF-Q II



Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	950 m/z	Set Collision Cell RF	150.0 Vpp	Set Divert Valve	Source

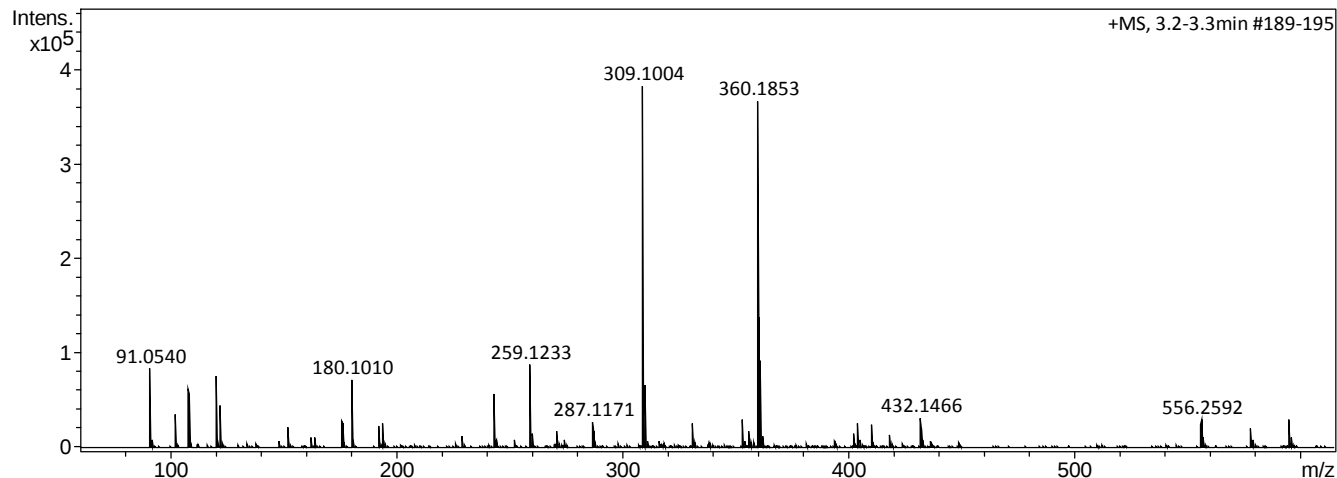

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
578.2404	1	C33H34FN3NaO4	578.2426	3.7	13.7	2	35.51	17.5	even	ok