

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\Eve\US-44.d
Method Tune_low_format 210120.m
Sample Name US-44
Comment SV: MeOH
Cecilia Attorressi

Acquisition Date 8/23/2022 1:04:19 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	950 m/z	Set Collision Cell RF	150.0 Vpp	Set Divert Valve	Source

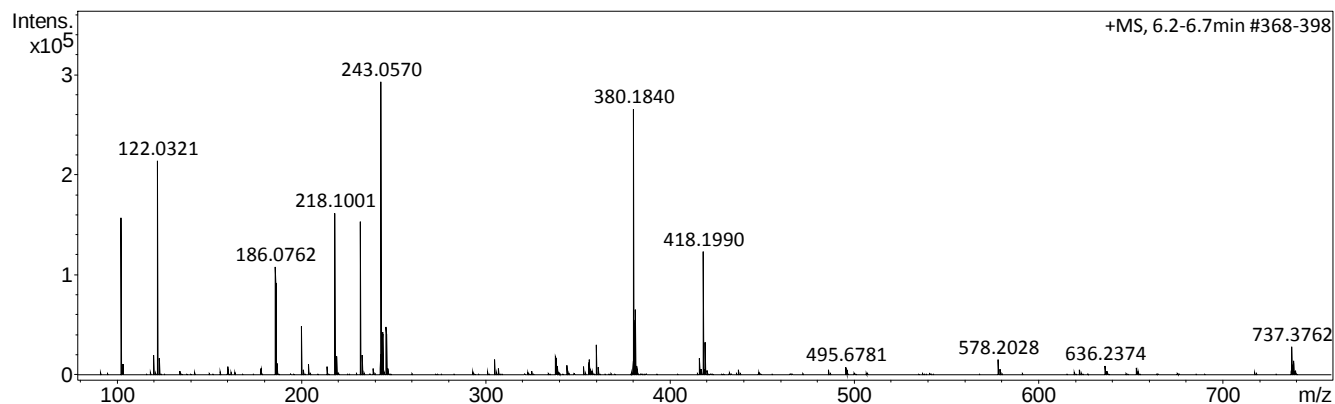

#	m/z	I	I %
1	102.1213	157067	53.8
2	103.1245	11096	3.8
3	120.0723	20003	6.8
4	122.0321	213252	73.0
5	123.0346	16727	5.7
6	186.0762	107509	36.8
7	187.0795	11697	4.0
8	200.0913	48602	16.6
9	204.0840	10719	3.7
10	218.1001	161142	55.2
11	219.1023	18873	6.5
12	232.1145	152903	52.4
13	233.1178	20175	6.9
14	243.0570	292035	100.0
15	244.0608	42617	14.6
16	246.1284	47894	16.4
17	304.9757	15302	5.2
18	338.1133	18612	6.4
19	339.1208	9131	3.1
20	344.1691	10027	3.4
21	356.1830	15651	5.4
22	360.1616	30348	10.4
23	380.1840	265069	90.8
24	381.1878	65309	22.4
25	416.1857	16865	5.8
26	418.1990	123151	42.2
27	419.2039	32673	11.2
28	578.2028	15329	5.2
29	737.3762	28417	9.7
30	738.3825	13925	4.8