

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\Eve\US-45 despues de calentar .d
Method Tune_low_formate 210120.m
Sample Name US-45 despues de calentar
Comment Cecilia

Acquisition Date 8/25/2022 4:00:47 PM
Operator ELB
Instrument / Ser# micrOTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	950 m/z	Set Collision Cell RF	150.0 Vpp	Set Divert Valve	Source

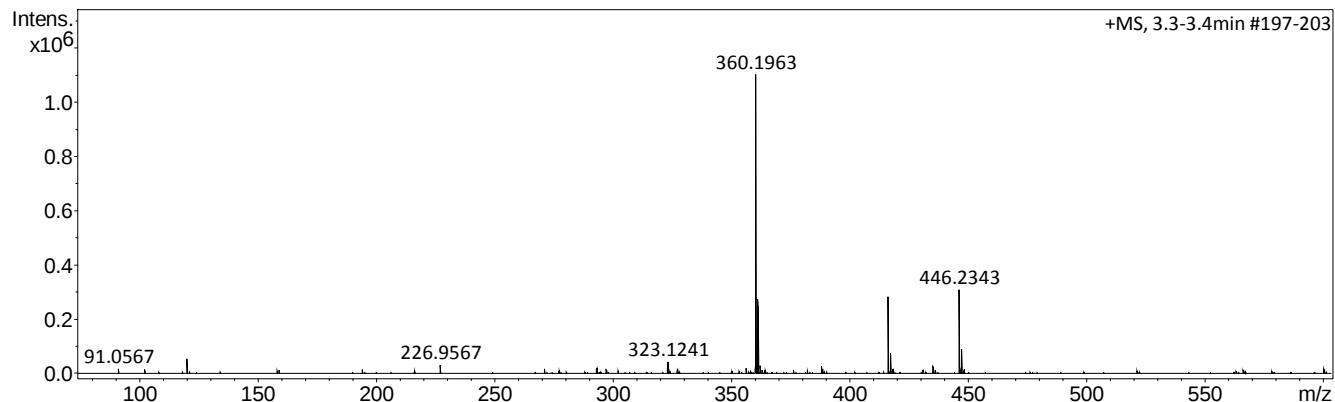

#	m/z	I	I %
1	91.0567	18446	1.7
2	102.1306	15730	1.4
3	120.0840	55633	5.1
4	158.9673	12606	1.1
5	194.1224	14834	1.3
6	226.9567	32103	2.9
7	271.1304	17747	1.6
8	293.1262	20900	1.9
9	297.1474	16212	1.5
10	323.1241	42919	3.9
11	327.1573	14848	1.3
12	356.2197	19978	1.8
13	360.1963	1101520	100.0
14	361.1989	272464	24.7
15	362.1995	29627	2.7
16	362.9329	12028	1.1
17	376.1882	13640	1.2
18	388.1916	27996	2.5
19	416.2233	281889	25.6
20	417.2275	76343	6.9
21	418.2208	14310	1.3
22	430.9226	12188	1.1
23	435.2385	26311	2.4
24	436.2342	13813	1.3
25	446.2343	308014	28.0
26	447.2371	89129	8.1
27	448.2385	14314	1.3
28	566.2622	12290	1.1
29	600.2986	16695	1.5
30	614.3144	11921	1.1