

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\Eve\US-45.d
Method Tune_low_format 210120.m
Sample Name US-45
Comment SV: MeOH
Cecilia Attorressi

Acquisition Date 8/23/2022 1:30:02 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	950 m/z	Set Collision Cell RF	150.0 Vpp	Set Divert Valve	Source

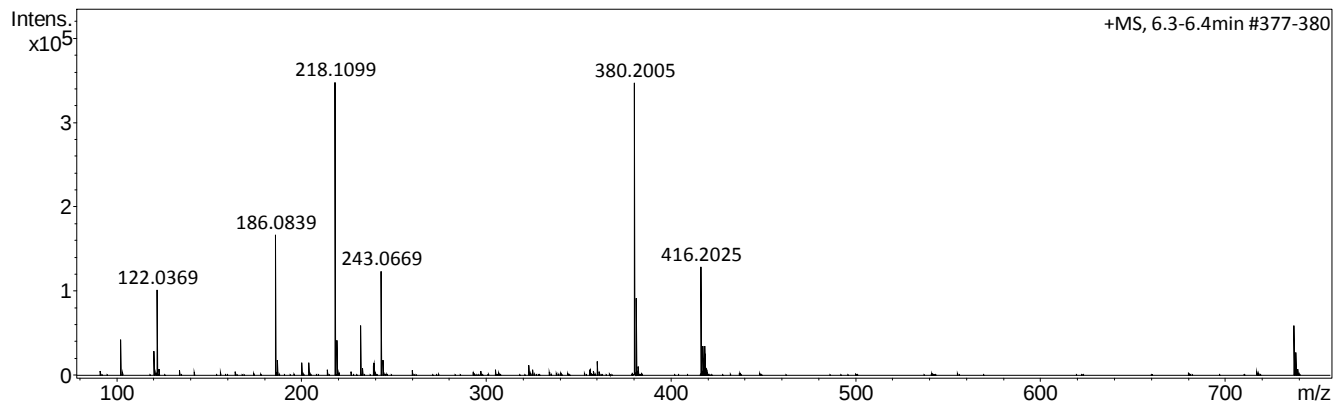

#	m/z	I	I %
1	102.1248	42215	12.2
2	120.0776	29168	8.4
3	122.0369	101073	29.1
4	123.0392	7793	2.2
5	186.0839	166746	48.1
6	187.0863	18429	5.3
7	200.1077	15325	4.4
8	204.0936	15529	4.5
9	214.1354	7198	2.1
10	218.1099	346962	100.0
11	219.1128	41656	12.0
12	232.1254	59114	17.0
13	233.1285	8162	2.4
14	239.1478	14610	4.2
15	243.0669	123527	35.6
16	244.0684	18474	5.3
17	323.1075	12286	3.5
18	325.1227	6694	1.9
19	356.2015	6739	1.9
20	360.1763	16922	4.9
21	380.2005	346382	99.8
22	381.2020	91465	26.4
23	382.2044	11001	3.2
24	416.2025	128437	37.0
25	417.2053	34521	9.9
26	418.2168	35253	10.2
27	419.2204	8347	2.4
28	737.4159	59012	17.0
29	738.4196	27704	8.0
30	739.4243	7996	2.3