

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UC-1_P1-C-8_01_8134.d
Method lc_qtof_directospos.m
Sample Name UC-1
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 4:10:05 PM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

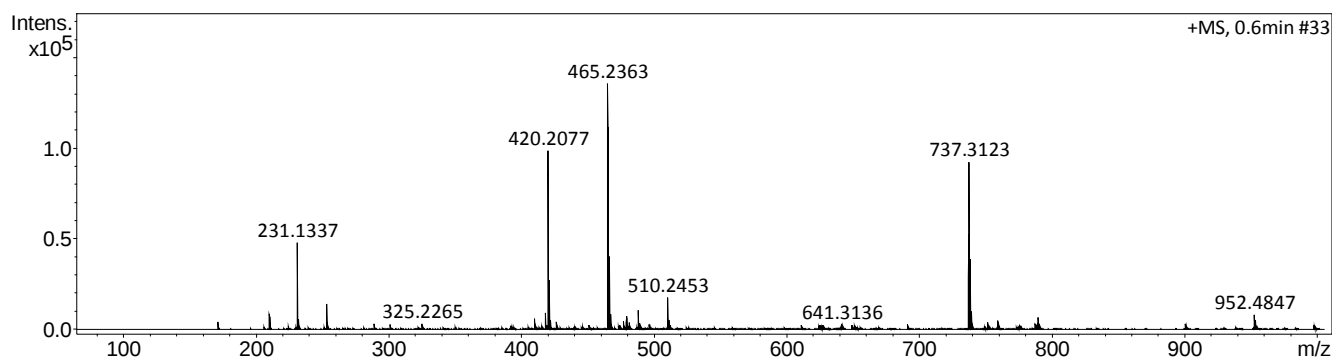

#	m/z	I	I %
1	171.1127	4399	3.2
2	210.1108	8409	6.2
3	231.1337	47902	35.4
4	232.1353	5611	4.1
5	253.1152	14014	10.4
6	325.2265	3285	2.4
7	410.1669	5873	4.3
8	418.1899	9014	6.7
9	420.2077	98397	72.7
10	421.2090	27189	20.1
11	422.2006	4904	3.6
12	426.2586	4058	3.0
13	465.2363	135397	100.0
14	466.2379	40062	29.6
15	467.2367	8284	6.1
16	477.2321	4654	3.4
17	479.2528	7413	5.5
18	481.2454	3745	2.8
19	488.2576	10576	7.8
20	489.2655	3457	2.6
21	510.2453	17442	12.9
22	511.2454	5280	3.9
23	737.3123	91973	67.9
24	738.3144	38550	28.5
25	739.3233	9797	7.2
26	751.4319	3938	2.9
27	759.2995	4820	3.6
28	789.4150	6777	5.0
29	952.4847	8089	6.0
30	953.4895	5164	3.8