

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UC-1_P1-C-8_01_8134.d
Method lc_qtof_directospos.m
Sample Name UC-1
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 4:10:05 PM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

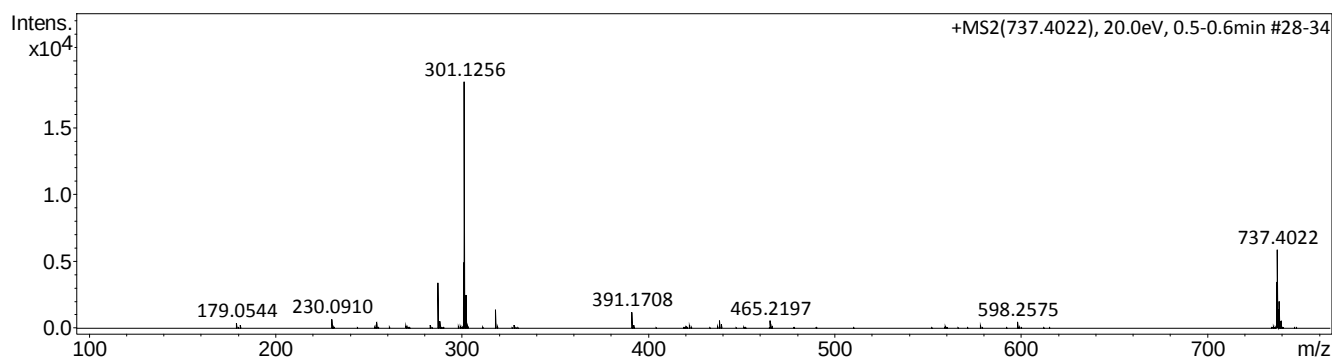

#	m/z	I	I %
1	179.0544	395	2.1
2	181.0712	259	1.4
3	230.0910	683	3.7
4	254.0894	447	2.4
5	270.0897	193	1.0
6	283.1153	239	1.3
7	287.1113	3411	18.5
8	288.1135	542	2.9
9	298.1404	178	1.0
10	299.1233	172	0.9
11	301.1256	18396	100.0
12	302.1307	2469	13.4
13	303.1303	235	1.3
14	318.0958	1373	7.5
15	319.0980	149	0.8
16	328.1129	260	1.4
17	391.1708	1205	6.6
18	392.1726	250	1.4
19	422.1580	220	1.2
20	437.1757	136	0.7
21	438.1509	602	3.3
22	439.1566	298	1.6
23	465.2197	606	3.3
24	466.2270	158	0.9
25	559.2275	172	0.9
26	578.2846	189	1.0
27	598.2575	478	2.6
28	737.4022	5896	32.1
29	738.4018	2001	10.9
30	739.4023	539	2.9