

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UC-1-sub_P1-C-9_01_8135.d
Method lc_qtof_directospos.m
Sample Name UC-1-sub
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 4:15:13 PM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

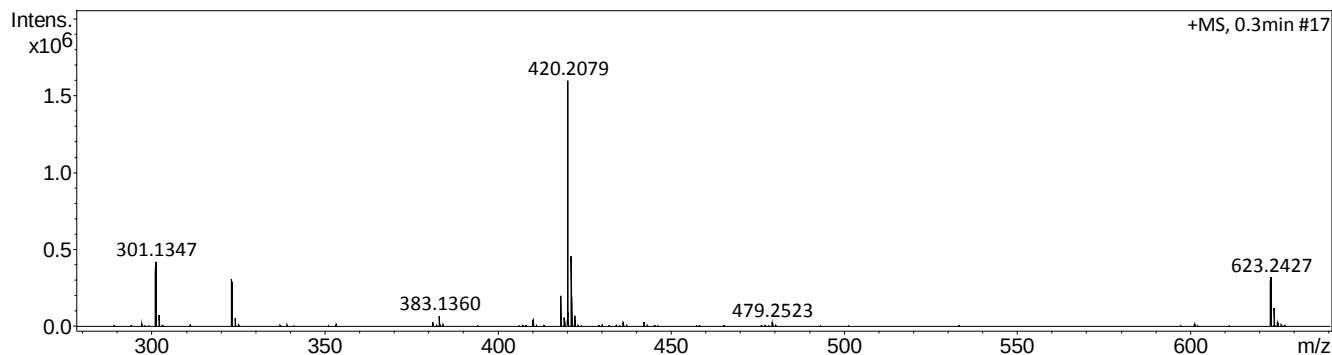

#	m/z	I	I %
1	297.1001	20949	1.3
2	301.1347	418457	26.2
3	302.1382	75887	4.8
4	303.1424	10518	0.7
5	323.1169	308452	19.3
6	324.1201	54603	3.4
7	325.1273	11181	0.7
8	339.1020	10663	0.7
9	353.2634	12856	0.8
10	381.2952	28248	1.8
11	383.1360	65480	4.1
12	384.1399	14156	0.9
13	407.1736	10273	0.6
14	410.1663	43910	2.8
15	411.1683	10614	0.7
16	418.1906	200349	12.6
17	419.1955	58259	3.7
18	420.2079	1595693	100.0
19	421.2096	454433	28.5
20	422.2091	68877	4.3
21	434.2168	9674	0.6
22	436.2002	24571	1.5
23	442.1892	29999	1.9
24	479.2523	25560	1.6
25	601.2594	14086	0.9
26	623.2427	317957	19.9
27	624.2469	120450	7.5
28	625.2529	23324	1.5
29	626.3081	11071	0.7
30	729.2803	12758	0.8