

Qualitative Compound Report

Analysis Info

Analysis Name D:\Data\ggc\UC-1-sub_P1-C-9_01_8135.d
Method lc_qtof_directospos.m
Sample Name UC-1-sub
Comment Sv: DCM + MeOH + HCOOH
Attoresi


Acquisition Date 10/17/2023 4:15:13 PM

Operator ELB
Instrument micrOTOF-Q II



Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

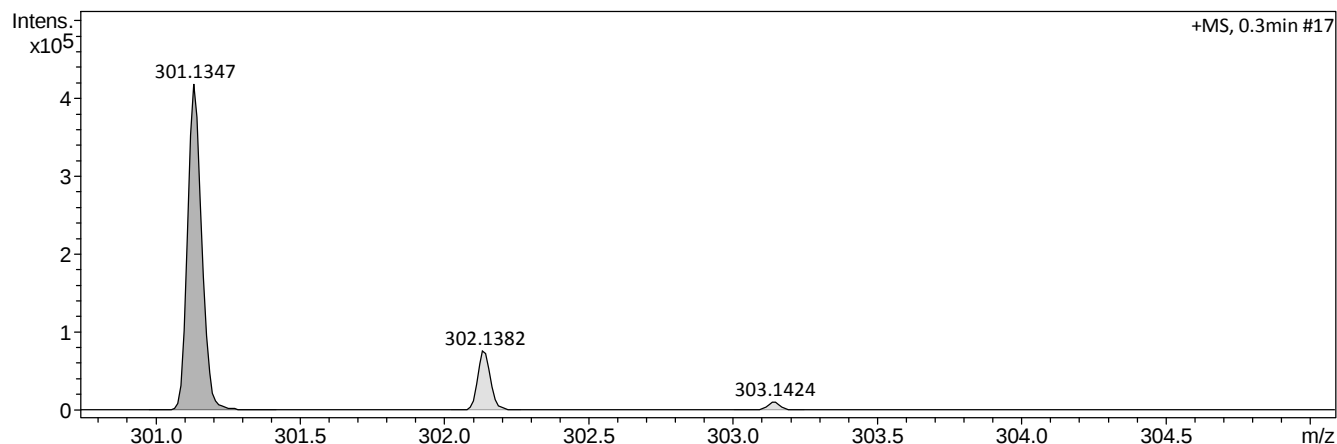

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
301.1347	1	C17H18FN2O2	301.1347	-0.2	7.5	1	100.00	9.5	even	ok