

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UC-2_P1-D-1_01_8136.d
Method lc_qtof_directospos.m
Sample Name UC-2
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 4:20:23 PM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

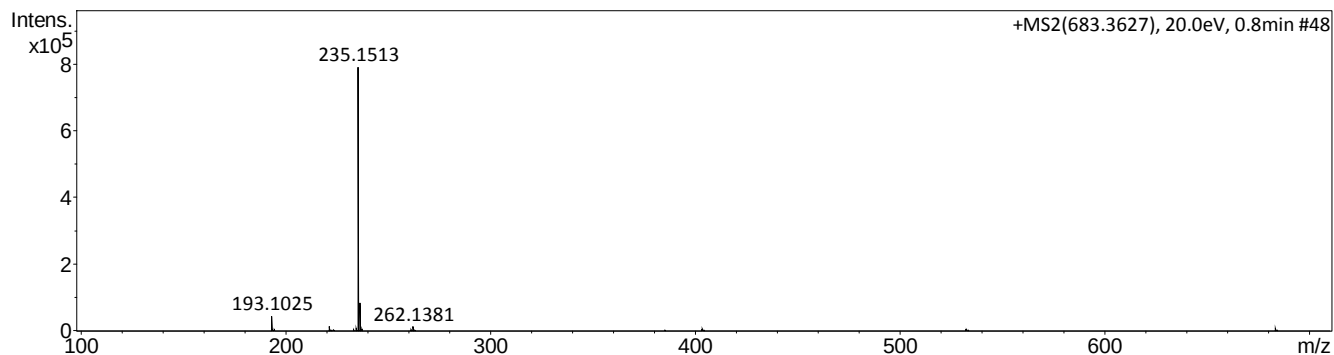

#	m/z	I	I %
1	193.1025	43696	5.5
2	194.1043	4099	0.5
3	217.1380	879	0.1
4	221.1336	14021	1.8
5	222.1360	1381	0.2
6	223.1490	1379	0.2
7	233.1338	2981	0.4
8	234.1416	8577	1.1
9	235.1513	788752	100.0
10	236.1537	83678	10.6
11	237.1569	5364	0.7
12	261.1288	2951	0.4
13	262.1381	13667	1.7
14	263.1422	1375	0.2
15	385.2090	1650	0.2
16	403.2107	6562	0.8
17	404.2160	1216	0.2
18	532.2963	4273	0.5
19	533.2982	1045	0.1
20	683.3627	8023	1.0
21	684.3686	2269	0.3