

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UC-2_P1-D-1_01_8206.d
Method lc_qtof_directospos mrm atorressi 683.m
Sample Name UC-2
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/25/2023 10:07:18 AM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

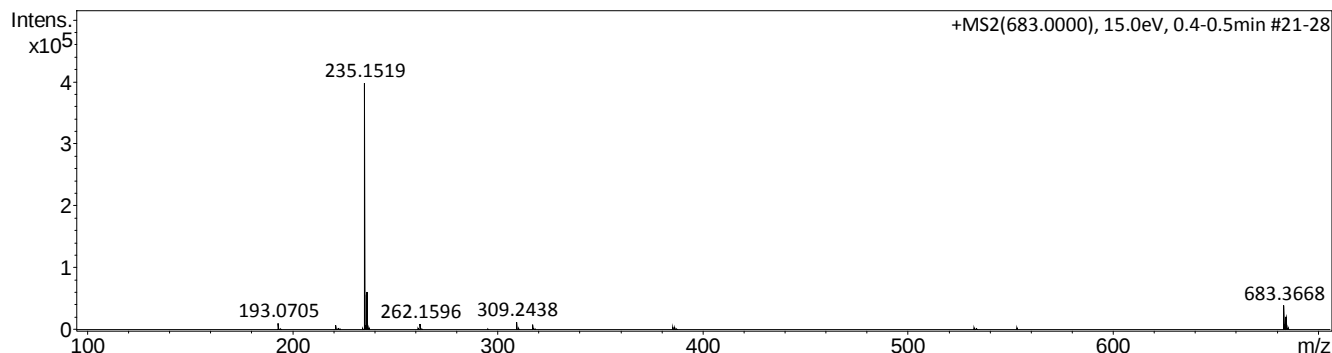

#	m/z	I	I %
1	193.0705	10768	2.7
2	194.0733	1226	0.3
3	221.1242	7709	1.9
4	222.1293	1021	0.3
5	223.1420	1090	0.3
6	233.1340	753	0.2
7	234.1418	2487	0.6
8	235.1519	397284	100.0
9	236.1557	61159	15.4
10	237.1583	3469	0.9
11	261.1510	2320	0.6
12	262.1596	9290	2.3
13	263.1626	1643	0.4
14	295.2180	939	0.2
15	309.2438	12582	3.2
16	310.2492	2552	0.6
17	317.2149	8829	2.2
18	318.2170	959	0.2
19	341.3439	527	0.1
20	385.3030	4749	1.2
21	386.3101	3428	0.9
22	387.3123	1152	0.3
23	532.3969	3500	0.9
24	533.3982	1280	0.3
25	553.2976	3244	0.8
26	560.3796	478	0.1
27	681.4102	462	0.1
28	683.3668	38882	9.8
29	684.3706	20728	5.2
30	685.3689	3009	0.8