

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UC-3_P1-D-2_01_8137.d
Method lc_qtof_directospos.m
Sample Name UC-3
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 4:25:30 PM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

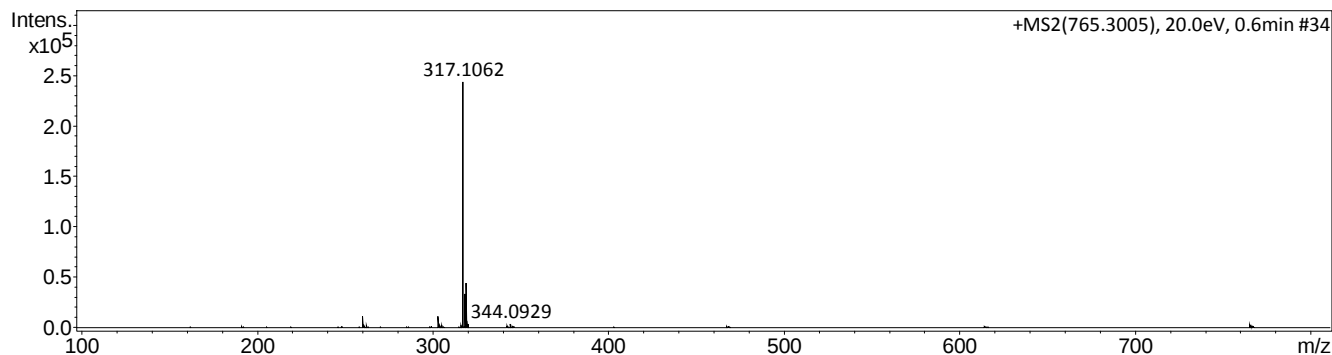

#	m/z	I	I %
1	162.0586	616	0.3
2	191.0821	1416	0.6
3	219.0769	510	0.2
4	246.0700	619	0.3
5	260.0846	11061	4.5
6	261.0871	1310	0.5
7	262.0793	2236	0.9
8	299.1008	331	0.1
9	303.0891	11175	4.6
10	304.0907	1659	0.7
11	305.0878	2668	1.1
12	315.0907	340	0.1
13	316.0985	2684	1.1
14	317.1062	243483	100.0
15	318.1082	33601	13.8
16	319.1038	44270	18.2
17	320.1051	3565	1.5
18	342.1422	1551	0.6
19	343.0892	468	0.2
20	344.0929	3792	1.6
21	345.0892	826	0.3
22	346.0898	812	0.3
23	403.1976	732	0.3
24	467.1617	863	0.4
25	614.2399	873	0.4
26	765.3005	2891	1.2
27	765.5328	851	0.3
28	766.3053	1322	0.5
29	766.5224	416	0.2
30	767.3074	834	0.3