

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UC-3-sub-1_P1-D-3_01_8138.d
Method lc_qtof_directospos.m
Sample Name UC-3-sub-1
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 4:30:37 PM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

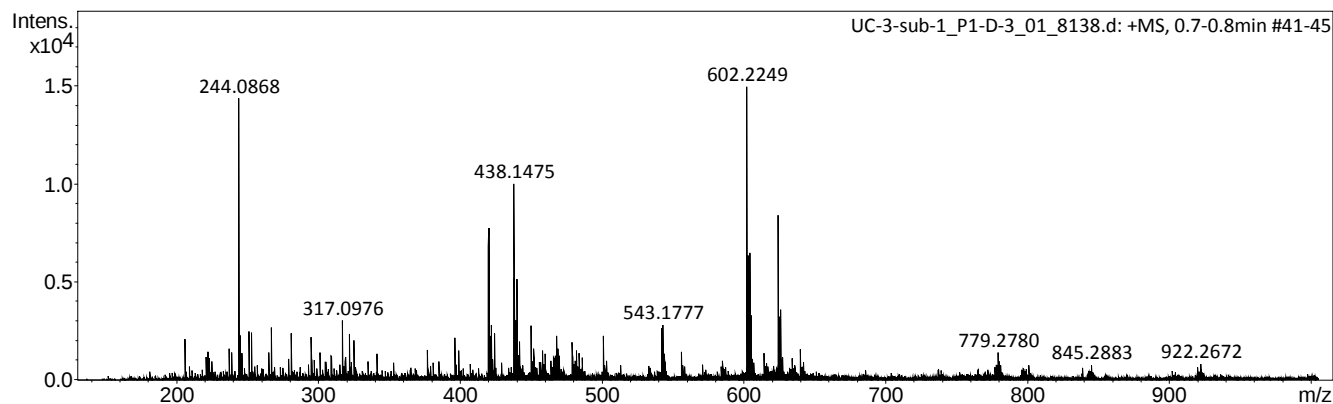

#	m/z	I	I %
1	206.1097	2084	14.0
2	244.0868	14357	96.2
3	245.0875	2266	15.2
4	251.1502	2096	14.0
5	253.1027	2412	16.2
6	267.1208	2657	17.8
7	281.1325	2391	16.0
8	295.1473	2183	14.6
9	317.0976	3040	20.4
10	322.0392	2327	15.6
11	396.3701	2158	14.5
12	420.1500	7754	52.0
13	421.1574	2241	15.0
14	422.1410	2806	18.8
15	424.4032	2363	15.8
16	438.1475	9986	66.9
17	439.1502	3013	20.2
18	440.1358	5149	34.5
19	450.1478	2779	18.6
20	468.1531	2244	15.0
21	501.1625	2242	15.0
22	542.1770	2644	17.7
23	543.1777	2803	18.8
24	602.2249	14924	100.0
25	603.2129	6333	42.4
26	604.2184	6480	43.4
27	605.2022	3298	22.1
28	624.2068	8383	56.2
29	625.2087	3208	21.5
30	626.2033	3579	24.0