

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UC-3-sub-1_P1-D-3_01_8138.d
Method lc_qtof_directospos.m
Sample Name UC-3-sub-1
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 4:30:37 PM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

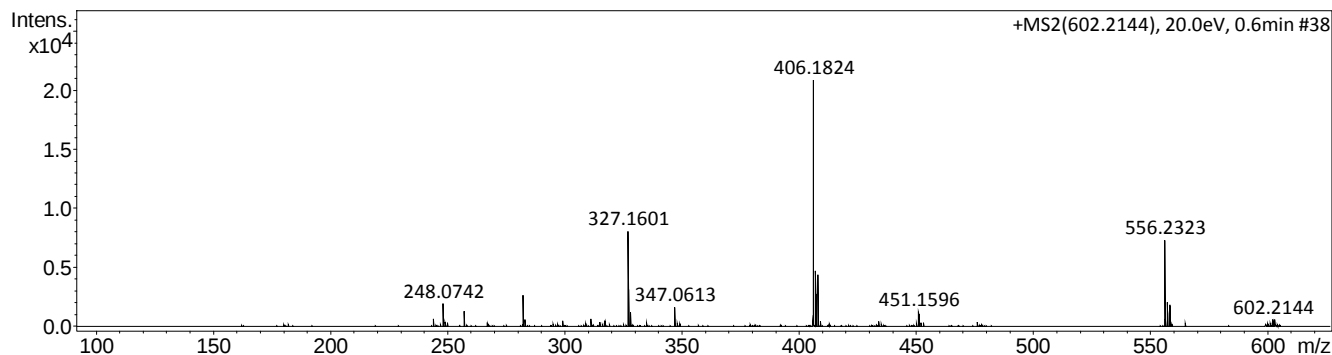

#	m/z	I	I %
1	244.0877	668	3.2
2	248.0742	1939	9.3
3	249.0715	372	1.8
4	250.0730	337	1.6
5	257.1192	1324	6.4
6	282.1763	2635	12.6
7	283.1775	599	2.9
8	299.1654	492	2.4
9	311.1655	627	3.0
10	315.0812	372	1.8
11	317.0975	494	2.4
12	327.1601	8028	38.5
13	328.1647	1211	5.8
14	335.0608	306	1.5
15	347.0613	1607	7.7
16	348.0649	290	1.4
17	406.1824	20839	100.0
18	407.1816	4699	22.5
19	408.1770	4376	21.0
20	409.1828	413	2.0
21	434.1542	425	2.0
22	451.1596	1243	6.0
23	452.1585	313	1.5
24	453.1581	339	1.6
25	476.1889	360	1.7
26	556.2323	7306	35.1
27	557.2361	2073	9.9
28	558.2287	1832	8.8
29	602.2144	619	3.0
30	603.1721	569	2.7