

Qualitative Compound Report

Analysis Info

Analysis Name D:\Data\ggc\UC-3-sub-1_P1-D-3_01_8138.d
Method lc_qtof_directospos.m
Sample Name UC-3-sub-1
Comment Sv: DCM + MeOH + HCOOH
Attoresi


Acquisition Date 10/17/2023 4:30:37 PM

Operator ELB
Instrument micrOTOF-Q II



Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

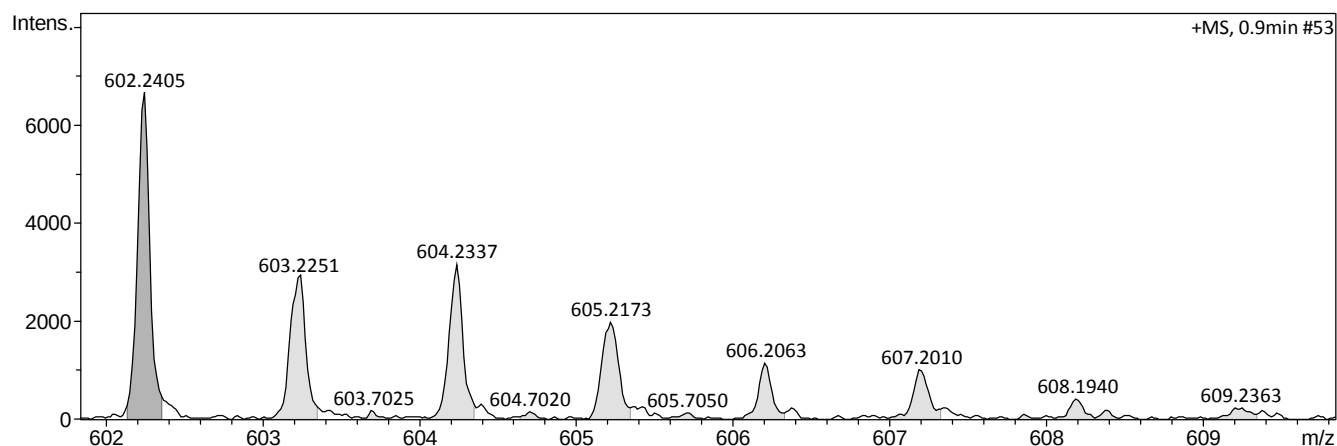

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdB	e ⁻ Conf	N-Rule
602.2405	1	C34H37ClN3O5	602.2416	1.9	185.8	2	0.05	17.5	even	ok