

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UC-4-sub-1_P1-D-4_01_8139.d
Method lc_qtof_directospos.m
Sample Name UC-4-sub-1
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 4:35:45 PM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

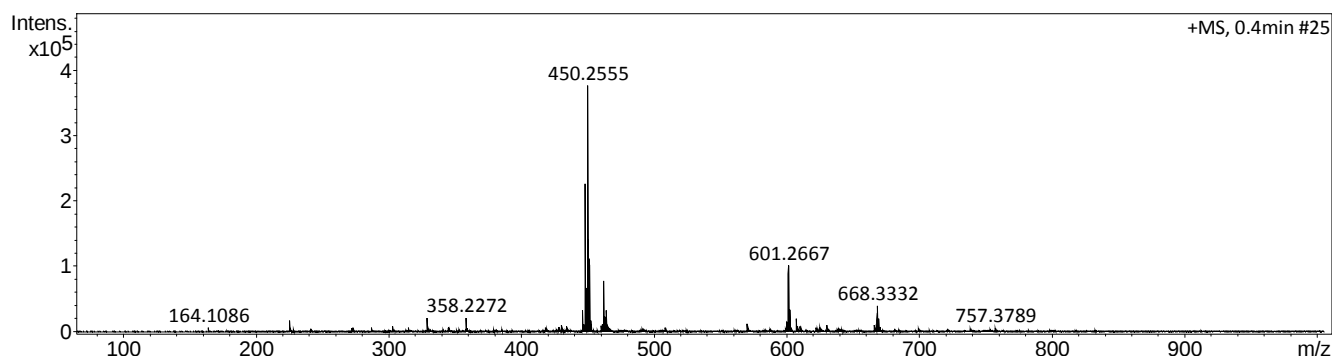

#	m/z	I	I %
1	225.1391	16698	4.4
2	303.1513	8587	2.3
3	329.1653	20586	5.5
4	358.2272	21451	5.7
5	430.2496	9907	2.6
6	434.2220	8513	2.3
7	446.2253	33115	8.8
8	447.2283	11040	2.9
9	448.2405	225805	60.0
10	449.2431	66656	17.7
11	450.2555	376322	100.0
12	451.2573	111501	29.6
13	452.2599	17275	4.6
14	460.2375	9260	2.5
15	461.2426	11012	2.9
16	462.2545	77198	20.5
17	463.2581	23218	6.2
18	464.2374	32846	8.7
19	465.2367	9600	2.6
20	570.3106	12643	3.4
21	600.2878	15142	4.0
22	601.2667	100581	26.7
23	602.2683	34143	9.1
24	607.3091	19632	5.2
25	608.3122	8117	2.2
26	610.3086	7934	2.1
27	630.2984	10016	2.7
28	666.3217	10115	2.7
29	668.3332	39338	10.5
30	669.3388	20194	5.4