

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UC-4-sub-1_P1-D-4_01_8139.d
Method lc_qtof_directospos.m
Sample Name UC-4-sub-1
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 4:35:45 PM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

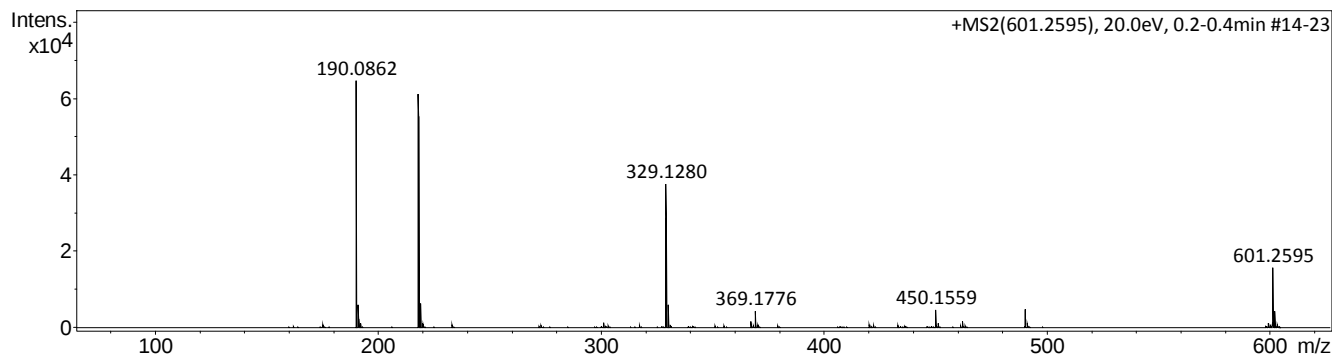

#	m/z	I	I %
1	175.0632	863	1.3
2	190.0862	64538	100.0
3	191.0883	5916	9.2
4	192.0975	1096	1.7
5	218.0807	61114	94.7
6	219.0834	6375	9.9
7	220.0891	904	1.4
8	233.0851	834	1.3
9	273.1379	555	0.9
10	301.1325	1378	2.1
11	317.1274	699	1.1
12	329.1280	37494	58.1
13	330.1297	5993	9.3
14	331.1315	499	0.8
15	367.2001	1675	2.6
16	369.1776	4366	6.8
17	370.1833	585	0.9
18	420.1854	786	1.2
19	422.1670	580	0.9
20	433.2228	669	1.0
21	450.1559	4663	7.2
22	451.1578	1118	1.7
23	462.2192	1579	2.4
24	490.2115	4795	7.4
25	491.2146	1127	1.7
26	599.2634	1060	1.6
27	600.2718	696	1.1
28	601.2595	15586	24.1
29	602.2634	4366	6.8
30	603.2716	771	1.2