

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UC-4-sub-2_P1-D-5_01_8140.d
Method lc_qtof_directospos.m
Sample Name UC-4-sub-2
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 4:40:53 PM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

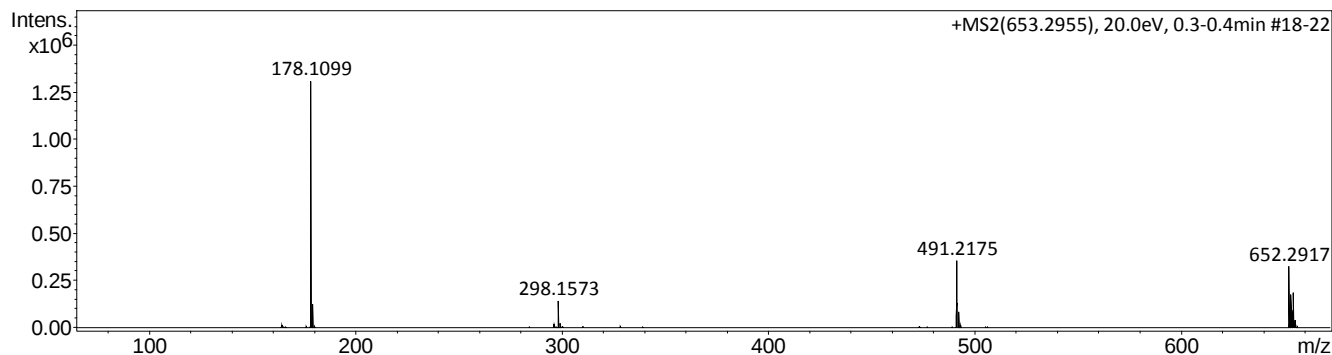

#	m/z	I	I %
1	164.0949	12773	1.0
2	166.1087	1922	0.1
3	176.0935	5438	0.4
4	178.1099	1303211	100.0
5	179.1123	124843	9.6
6	180.1139	5660	0.4
7	296.1419	14558	1.1
8	297.1456	2181	0.2
9	298.1573	140102	10.8
10	299.1608	21430	1.6
11	300.1618	1927	0.1
12	310.1197	2503	0.2
13	328.1303	4900	0.4
14	339.1225	2145	0.2
15	473.2072	2313	0.2
16	489.2035	1328	0.1
17	491.2175	355025	27.2
18	492.2204	84957	6.5
19	493.2237	11745	0.9
20	505.2287	3251	0.2
21	652.2917	322356	24.7
22	653.2955	173889	13.3
23	654.3044	186145	14.3
24	655.3069	40716	3.1
25	656.3077	7120	0.5