

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UC-4-sub-2_P1-D-5_01_8140.d
Method lc_qtof_directospos.m
Sample Name UC-4-sub-2
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 4:40:53 PM

Operator ELB
Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

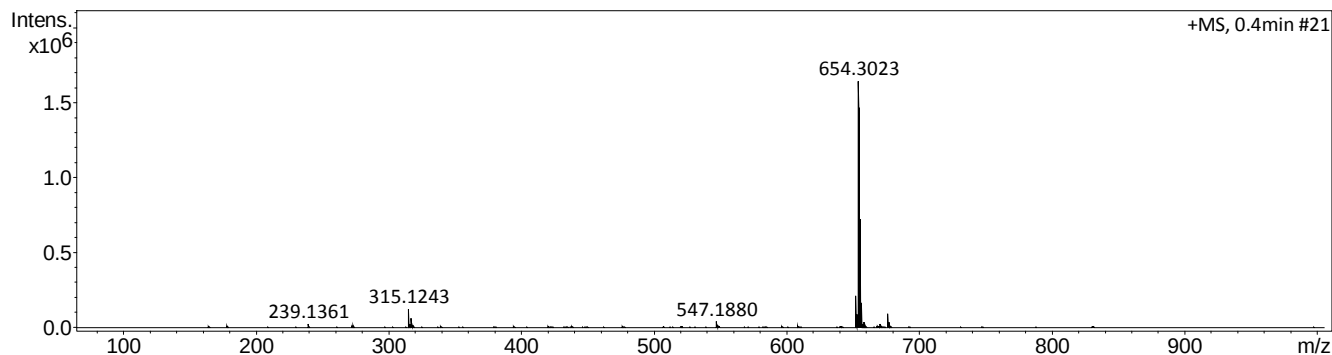

#	m/z	I	I %
1	164.0935	9642	0.6
2	178.1076	11527	0.7
3	239.1361	25115	1.5
4	272.1414	8765	0.5
5	273.1185	15492	0.9
6	315.1243	121768	7.4
7	316.1277	23845	1.5
8	317.1383	61833	3.8
9	318.1406	11085	0.7
10	420.1541	7205	0.4
11	438.1615	9145	0.6
12	476.1950	9482	0.6
13	547.1880	40794	2.5
14	548.1883	13322	0.8
15	596.2404	7995	0.5
16	608.2541	9867	0.6
17	652.2858	209665	12.8
18	653.2906	90108	5.5
19	654.3023	1640026	100.0
20	655.3045	719609	43.9
21	656.3063	163271	10.0
22	657.3080	22981	1.4
23	658.2949	35987	2.2
24	659.2981	13546	0.8
25	668.3053	9621	0.6
26	670.2954	24663	1.5
27	671.2961	9024	0.6
28	676.2826	93379	5.7
29	677.2826	36589	2.2
30	678.2857	8959	0.5