

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\UC-5_P1-F-2_01_8951.d
 Method lc_qtof_directospos.m
 Sample Name UC-5
 Comment Sv: MeOH + HCOOH
 Cecilia

Acquisition Date 10/4/2024 9:46:34 a. m.

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

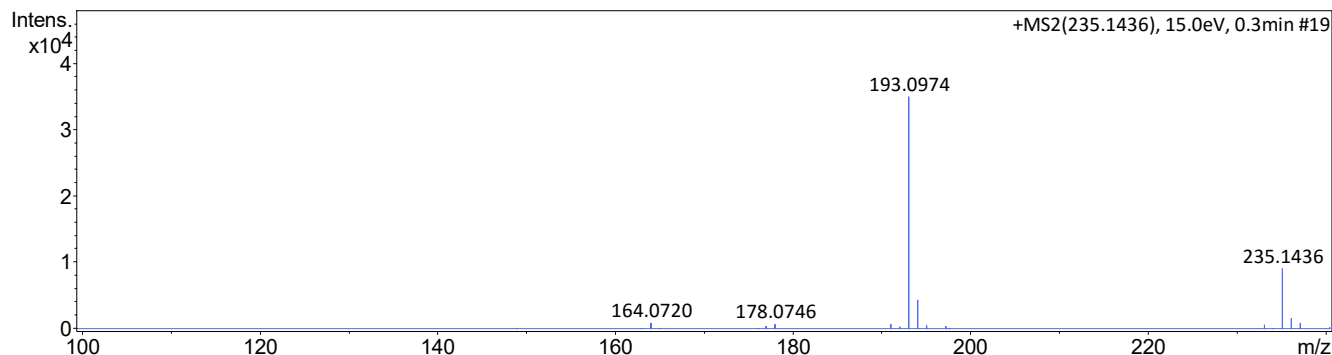

#	m/z	I	I %
1	149.0416	71	0.2
2	163.0889	145	0.4
3	164.0720	887	2.5
4	165.0688	107	0.3
5	176.0984	77	0.2
6	177.0675	371	1.1
7	178.0746	716	2.0
8	179.0989	48	0.1
9	190.0738	48	0.1
10	191.0836	643	1.8
11	192.0880	271	0.8
12	193.0974	34982	100.0
13	194.1000	4371	12.5
14	195.1042	510	1.5
15	197.2694	414	1.2
16	197.3279	88	0.3
17	197.4507	80	0.2
18	197.7352	144	0.4
19	203.1045	45	0.1
20	204.1136	53	0.2
21	233.1308	615	1.8
22	234.1261	157	0.4
23	235.1436	9048	25.9
24	236.1464	1578	4.5
25	237.1643	874	2.5
26	238.1744	53	0.2
27	240.5327	201	0.6
28	240.6056	152	0.4
29	240.7376	112	0.3
30	838.7523	260	0.7