

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\UC-6_P1-F-3_01_8957.d
 Method lc_qtof_directospos mrm atorressi uc-5.m
 Sample Name UC-6
 Comment Sv: MeOH + HCOOH
 Cecilia

Acquisition Date 10/4/2024 11:01:14 a. m.

Operator ELB
 Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

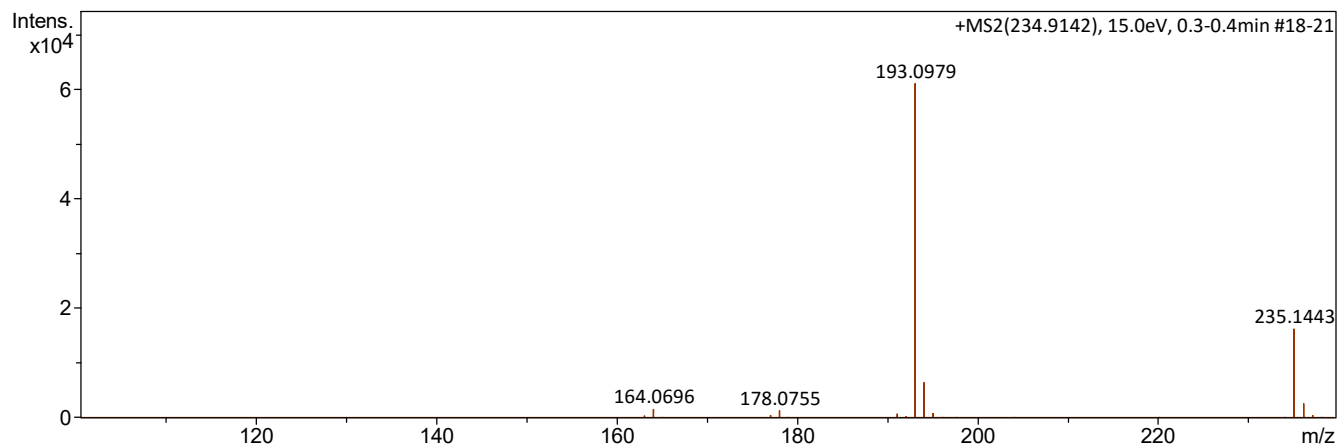

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
164.0696	1	C9H10NO2	164.0706	5.9	17.3	1	100.00	5.5	even	ok
193.0979	1	C10H13N2O2	193.0972	-3.9	6.9	1	100.00	5.5	even	ok
235.1443	1	C13H19N2O2	235.1441	-0.9	13.3	1	100.00	5.5	even	ok