

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\UC-6_P1-F-3_01_8957.d
 Method lc_qtof_directospos mrm atorressi uc-5.m
 Sample Name UC-6
 Comment Sv: MeOH + HCOOH
 Cecilia

Acquisition Date 10/4/2024 11:01:14 a. m.

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

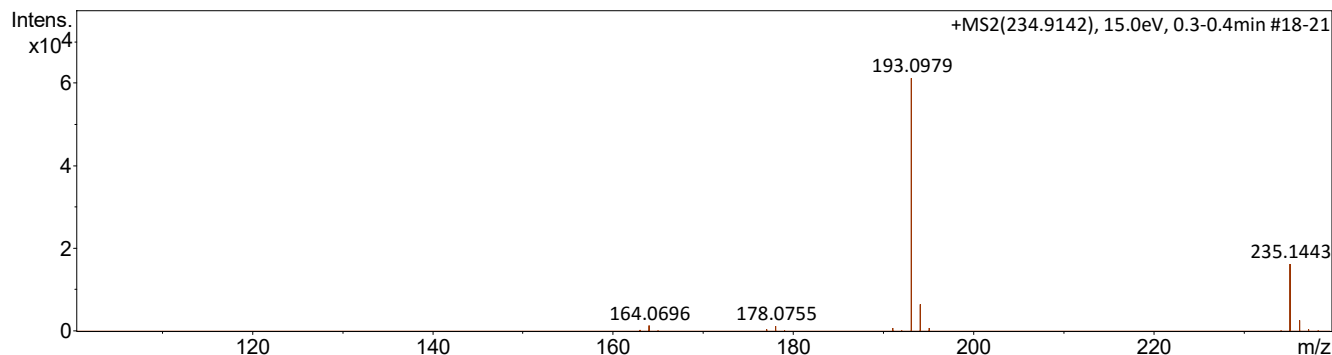

#	m/z	I	I %
1	163.0847	398	0.7
2	164.0696	1526	2.5
3	165.0734	203	0.3
4	175.0868	85	0.1
5	177.0692	519	0.8
6	178.0755	1300	2.1
7	179.0782	190	0.3
8	186.1101	95	0.2
9	191.0847	796	1.3
10	192.0878	285	0.5
11	193.0979	61122	100.0
12	194.1002	6487	10.6
13	195.1040	831	1.4
14	196.1437	138	0.2
15	197.2733	94	0.2
16	197.7349	125	0.2
17	202.1041	82	0.1
18	204.1231	136	0.2
19	216.1217	112	0.2
20	220.1180	136	0.2
21	232.1511	85	0.1
22	234.1444	162	0.3
23	235.1443	16227	26.5
24	236.1481	2625	4.3
25	237.1564	567	0.9
26	238.2210	157	0.3
27	239.8085	214	0.3
28	239.8907	307	0.5
29	240.5261	108	0.2
30	939.1086	206	0.3