

Qualitative Compound Report

Analysis Info


Analysis Name D:\Data\UC-6_P1-F-3_01_8957.d
Method lc_qtof_directospos mrm atorressi uc-5.m
Sample Name UC-6
Comment Sv: MeOH + HCOOH
Cecilia

Acquisition Date 10/4/2024 11:01:14 a. m.

Operator ELB
Instrument micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

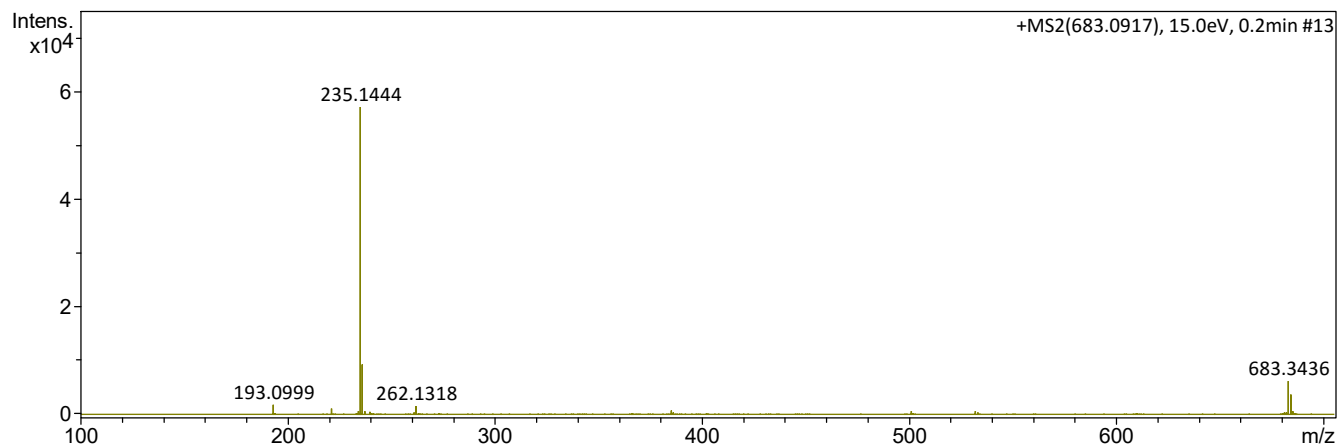

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdB	e ⁻ Conf	N-Rule
193.0999	1	C15H13	193.1012	6.4	33.1	1	100.00	9.5	even	ok
221.1295	1	C12H17N2O2	221.1285	-4.6	34.7	1	100.00	5.5	even	ok
235.1444	1	C13H19N2O2	235.1441	-1.1	6.5	1	100.00	5.5	even	ok
262.1318	1	C14H18N2O3	262.1312	-2.2	22.8	1	100.00	7.0	odd	ok
683.3436	1	C39H47N4O7	683.3439	0.5	71.7	1	100.00	18.5	even	ok