

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\UC-6_P1-F-3_01_8957.d
 Method lc_qtof_directospos mrm atorressi uc-5.m
 Sample Name UC-6
 Comment Sv: MeOH + HCOOH
 Cecilia

Acquisition Date 10/4/2024 11:01:14 a. m.

Operator ELB
 Instrument / Ser# microTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

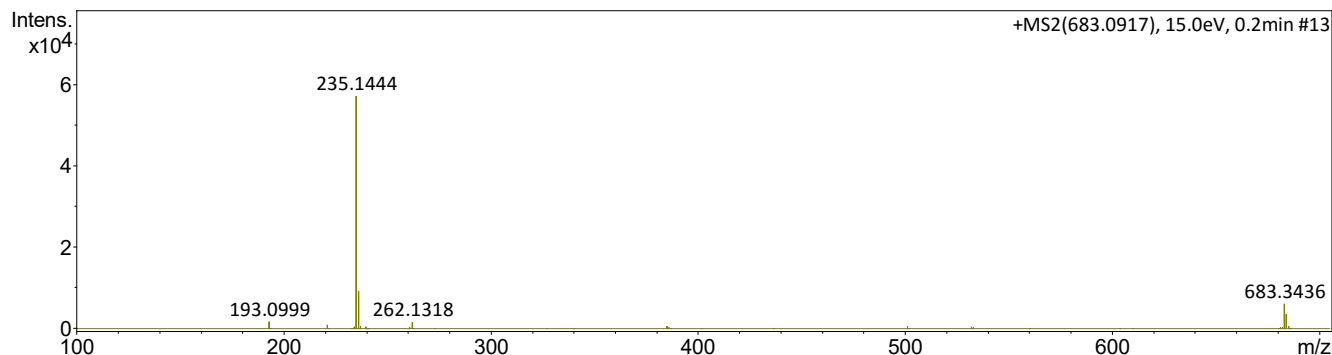

#	m/z	I	I %
1	193.0999	1780	3.1
2	194.0955	192	0.3
3	221.1295	1035	1.8
4	233.1291	167	0.3
5	234.1352	530	0.9
6	235.1444	57096	100.0
7	236.1464	9210	16.1
8	237.1499	597	1.0
9	239.8040	469	0.8
10	239.8868	407	0.7
11	261.1218	354	0.6
12	262.1318	1543	2.7
13	263.1376	189	0.3
14	273.1224	161	0.3
15	385.1980	639	1.1
16	386.1992	306	0.5
17	402.2080	157	0.3
18	501.2019	617	1.1
19	502.1939	186	0.3
20	532.2784	527	0.9
21	533.2769	338	0.6
22	610.2669	175	0.3
23	680.4061	240	0.4
24	681.3887	332	0.6
25	682.3777	373	0.7
26	683.3436	6207	10.9
27	684.3519	3636	6.4
28	685.3584	596	1.0
29	686.3678	157	0.3
30	939.0907	228	0.4