

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\UC-8_P1-F-5_01_8954.d
Method lc_qtof_directospos.m
Sample Name UC-8
Comment Sv: MeOH + HCOOH
Cecilia

Acquisition Date 10/4/2024 10:01:52 a. m.

Operator ELB
Instrument / Ser# micrOTOF-Q II

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

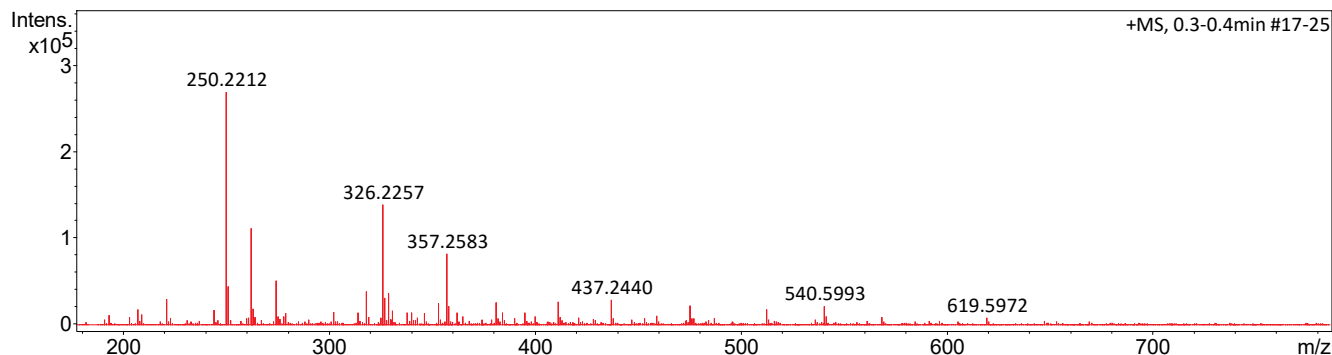

#	m/z	I	I %
1	207.1733	17631	6.6
2	221.1890	28982	10.8
3	244.1233	16951	6.3
4	250.2212	268604	100.0
5	251.2233	44309	16.5
6	262.2217	111524	41.5
7	263.2242	18039	6.7
8	274.3050	50588	18.8
9	279.2058	13234	4.9
10	302.3409	14203	5.3
11	314.2217	13458	5.0
12	318.3374	37851	14.1
13	326.2257	139041	51.8
14	327.2266	31066	11.6
15	329.0717	36308	13.5
16	331.0707	16334	6.1
17	338.1802	13457	5.0
18	340.3177	13993	5.2
19	353.3050	24566	9.1
20	357.2583	81571	30.4
21	358.2607	21454	8.0
22	362.3679	13580	5.1
23	381.3409	25360	9.4
24	384.3483	14112	5.3
25	395.2891	13932	5.2
26	411.2862	26428	9.8
27	437.2440	28226	10.5
28	475.2907	22138	8.2
29	512.5632	17715	6.6
30	540.5993	21324	7.9