

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\US-28_P1-F-1_01_2106.d
Method tune_pos_formatc lcms.m
Sample Name US-28
Comment Sv: agua + metanol
Dr. Oscar Varela

Acquisition Date 30/10/2019 2:31:54 p. m.

Operator GC
Instrument / Ser# micrOTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	8.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	200.0 Vpp	Set Divert Valve	Source

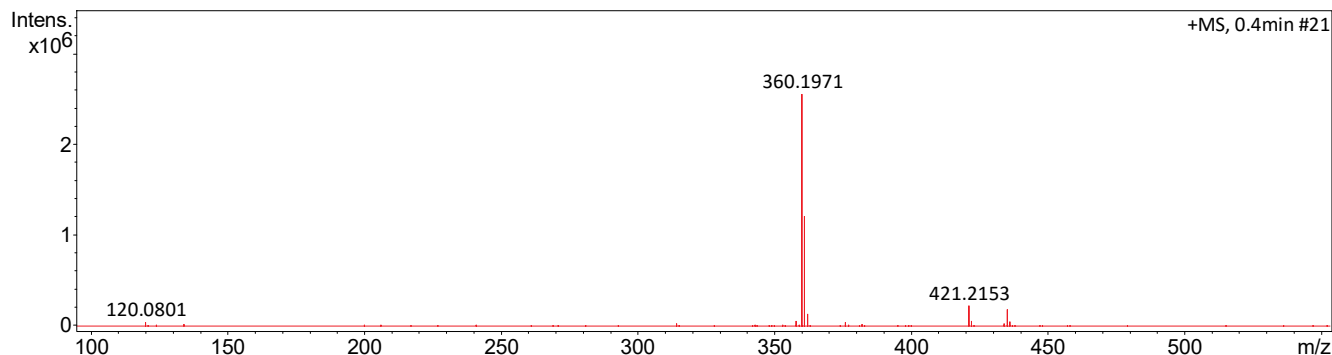

#	m/z	I	I %
1	120.0801	42792	1.7
2	124.0556	12120	0.5
3	134.0965	17063	0.7
4	200.0893	10164	0.4
5	206.1201	11420	0.4
6	241.1161	12308	0.5
7	314.2057	27005	1.1
8	343.1955	12570	0.5
9	353.1923	13789	0.5
10	358.1767	52548	2.1
11	359.1795	12224	0.5
12	360.1971	2548815	100.0
13	361.1957	1210896	47.5
14	362.1974	134144	5.3
15	363.2009	7972	0.3
16	376.1872	39656	1.6
17	377.1887	9464	0.4
18	382.1728	19677	0.8
19	398.1679	7966	0.3
20	421.2153	225369	8.8
21	422.2166	53095	2.1
22	434.2292	23853	0.9
23	435.2326	179408	7.0
24	436.2353	46466	1.8
25	447.2336	8795	0.3
26	457.2135	9172	0.4
27	685.3810	18519	0.7
28	686.3866	10483	0.4
29	819.4408	20039	0.8
30	820.4436	10140	0.4