

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\US-29_P1-F-2_01_2107.d
Method tune_pos_formatc lcms.m
Sample Name US-29
Comment Sv: agua + metanol
Dr. Oscar Varela

Acquisition Date 30/10/2019 2:37:01 p. m.

Operator GC
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	8.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	200.0 Vpp	Set Divert Valve	Source

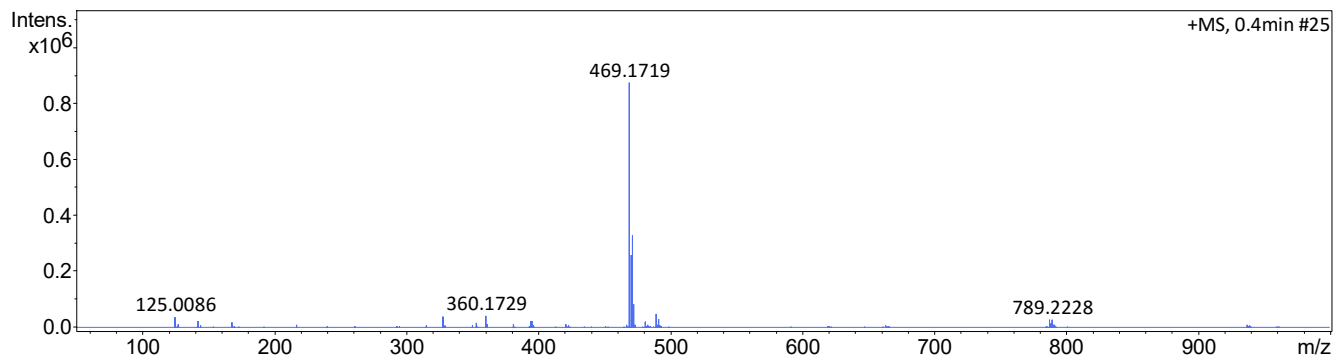

#	m/z	I	I %
1	125.0086	36238	4.1
2	127.0056	11108	1.3
3	142.0350	22441	2.6
4	168.0513	19432	2.2
5	328.1418	39638	4.5
6	353.2515	16323	1.9
7	360.1729	42026	4.8
8	361.1756	12101	1.4
9	381.2829	13209	1.5
10	394.1173	23822	2.7
11	394.6180	12072	1.4
12	395.1152	22443	2.6
13	395.6177	10618	1.2
14	421.0904	11993	1.4
15	467.1557	9351	1.1
16	469.1719	873898	100.0
17	470.1744	259244	29.7
18	471.1699	328414	37.6
19	472.1717	82373	9.4
20	473.1728	9598	1.1
21	481.1697	20991	2.4
22	483.1677	9422	1.1
23	489.1126	48981	5.6
24	490.1173	10936	1.3
25	491.1132	29515	3.4
26	787.2276	28561	3.3
27	788.2294	14387	1.6
28	789.2228	28896	3.3
29	790.2275	10800	1.2
30	937.3320	10935	1.3