

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\US-37_P1-D-1_01_5324.d
Method lc_qtof_directospos mrm atorresi.m
Sample Name US-37
Comment Sv: DCM + MeOH + HCOOH
Cecilia Attorresi

Acquisition Date 7/29/2022 9:12:33 AM
Operator ELB
Instrument / Ser# micrOTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

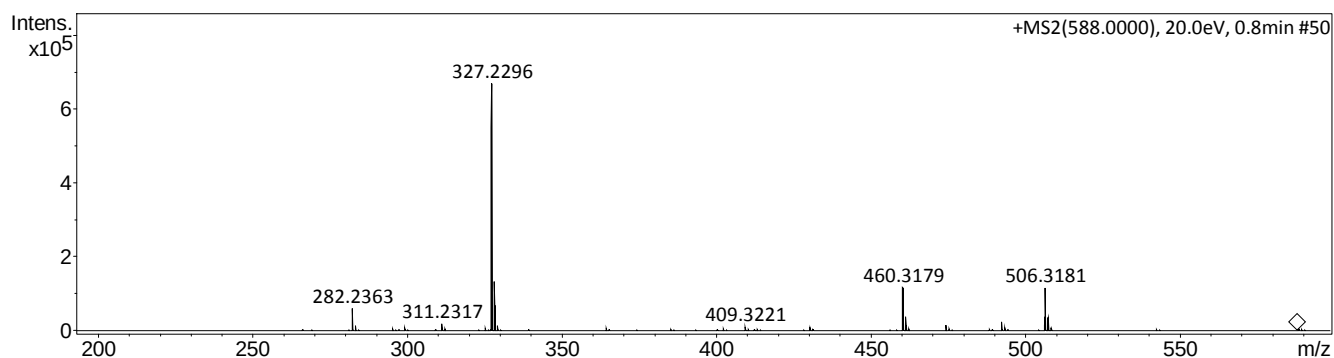

#	m/z	I	I %
1	282.2363	60182	9.0
2	283.2374	13781	2.1
3	295.2338	4078	0.6
4	299.2279	9080	1.4
5	311.2317	18068	2.7
6	312.2334	4018	0.6
7	325.2127	6832	1.0
8	327.2296	666970	100.0
9	328.2325	133019	19.9
10	329.2349	12983	1.9
11	364.3267	7208	1.1
12	385.2765	2741	0.4
13	402.2891	4948	0.7
14	409.3221	10331	1.5
15	410.3220	3414	0.5
16	413.2801	2506	0.4
17	430.2883	8576	1.3
18	431.2908	2531	0.4
19	460.3179	116246	17.4
20	461.3198	36961	5.5
21	462.3215	4587	0.7
22	474.2858	15278	2.3
23	475.2882	5023	0.8
24	492.2986	23253	3.5
25	493.3029	7407	1.1
26	506.3181	114935	17.2
27	507.3215	35343	5.3
28	508.3227	5947	0.9
29	588.4099	7465	1.1
30	589.4097	3076	0.5