

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\US-38_P1-D-2_01_5325.d
Method lc_qtof_directospos mrm atorressi.m
Sample Name US-38
Comment Sv: DCM + MeOH + HCOOH
Cecilia Attorresi

Acquisition Date 7/29/2022 9:17:39 AM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

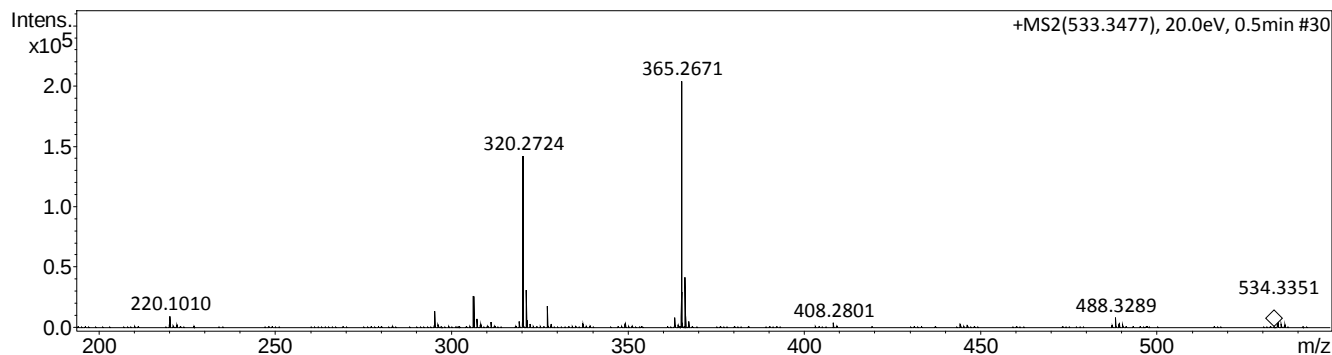

#	m/z	I	I %
1	220.1010	9435	4.6
2	222.0969	2218	1.1
3	295.2455	13434	6.6
4	296.2463	2598	1.3
5	306.2537	25714	12.6
6	307.2548	7295	3.6
7	308.2564	2332	1.1
8	311.2442	4816	2.4
9	319.2544	5235	2.6
10	320.2724	141718	69.7
11	321.2749	31259	15.4
12	322.2763	3197	1.6
13	327.2434	17960	8.8
14	328.2450	3247	1.6
15	337.2626	3185	1.6
16	349.2673	3688	1.8
17	363.2817	8214	4.0
18	364.2843	1965	1.0
19	365.2671	203452	100.0
20	366.2694	41808	20.5
21	367.2739	4959	2.4
22	408.2801	3951	1.9
23	444.3065	2331	1.1
24	487.3212	1355	0.7
25	488.3289	8207	4.0
26	489.3258	3380	1.7
27	490.3263	2682	1.3
28	534.3351	7629	3.7
29	535.3369	2887	1.4
30	536.3303	2320	1.1