

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\US-39_P1-D-3_01_5330.d
Method lc_qtof_directospos mrm atorresi.m
Sample Name US-39
Comment Sv: DCM + MeOH + HCOOH
Cecilia Attorresi

Acquisition Date 7/29/2022 9:43:12 AM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

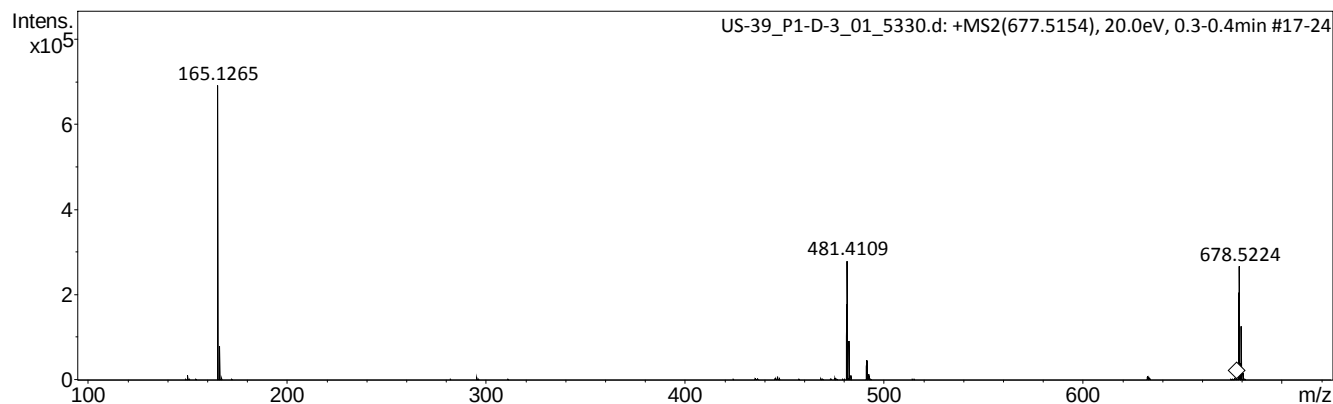

#	m/z	I	I %
1	150.0972	9852	1.4
2	165.1265	689422	100.0
3	166.1300	78602	11.4
4	167.1333	3798	0.6
5	172.1685	2244	0.3
6	282.2466	1810	0.3
7	295.2449	5529	0.8
8	424.3768	1921	0.3
9	435.3585	3078	0.4
10	445.3541	3705	0.5
11	446.3658	7940	1.2
12	447.3679	2410	0.3
13	468.4016	2667	0.4
14	469.3856	1787	0.3
15	473.3486	2050	0.3
16	475.3623	5187	0.8
17	476.3660	1722	0.2
18	481.4109	278295	40.4
19	482.4142	91557	13.3
20	483.4171	9877	1.4
21	491.3604	45654	6.6
22	492.3642	13904	2.0
23	632.5133	6914	1.0
24	633.5171	3335	0.5
25	674.5249	2033	0.3
26	675.5259	1852	0.3
27	676.5153	2484	0.4
28	678.5224	266542	38.7
29	679.5268	126200	18.3
30	680.5283	16457	2.4