

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\US-40_P1-D-4_01_5326.d
Method lc_qtof_directospos mrm atorressi.m
Sample Name US-40
Comment Sv: DCM + MeOH + HCOOH
Cecilia Attorresi

Acquisition Date 7/29/2022 9:22:47 AM
Operator ELB
Instrument / Ser# micrOTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

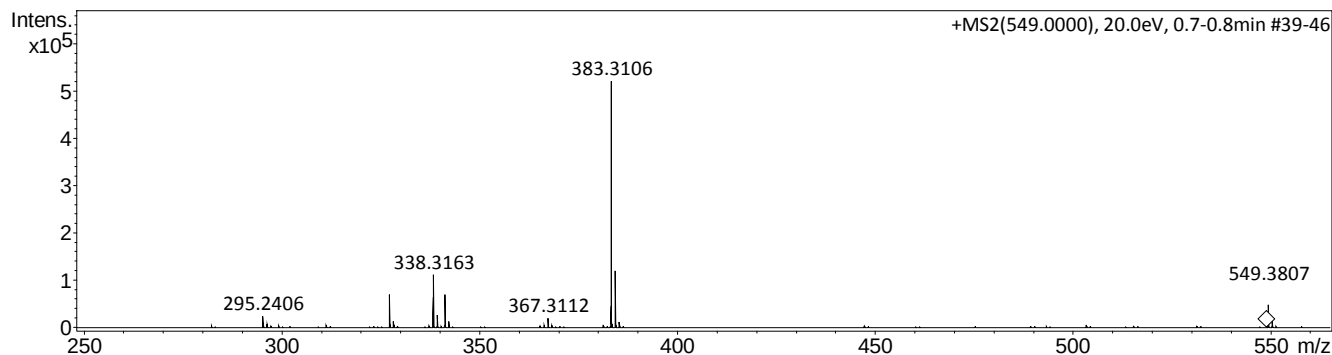

#	m/z	I	I %
1	282.2426	3724	0.7
2	295.2406	23948	4.6
3	296.2497	7035	1.4
4	297.2522	1761	0.3
5	299.2354	3969	0.8
6	311.2388	5323	1.0
7	327.2362	69145	13.3
8	328.2392	13055	2.5
9	337.2951	3223	0.6
10	338.3163	111936	21.5
11	339.3185	26189	5.0
12	340.3199	3033	0.6
13	341.2554	69310	13.3
14	342.2580	13787	2.7
15	365.3030	2350	0.5
16	366.3156	5260	1.0
17	367.3112	20494	3.9
18	368.3127	4990	1.0
19	381.2935	3523	0.7
20	383.3106	520097	100.0
21	384.3136	119776	23.0
22	385.3149	11728	2.3
23	447.3038	2504	0.5
24	493.3081	1901	0.4
25	503.3791	3420	0.7
26	515.3654	1753	0.3
27	531.3674	2536	0.5
28	549.3807	48710	9.4
29	550.3839	14748	2.8
30	551.3885	2394	0.5