

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\US-41_P1-D-5_01_5327.d
Method lc_qtof_directospos mrm atorressi.m
Sample Name US-41
Comment Sv: DCM + MeOH + HCOOH
Cecilia Attorresi

Acquisition Date 7/29/2022 9:27:53 AM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

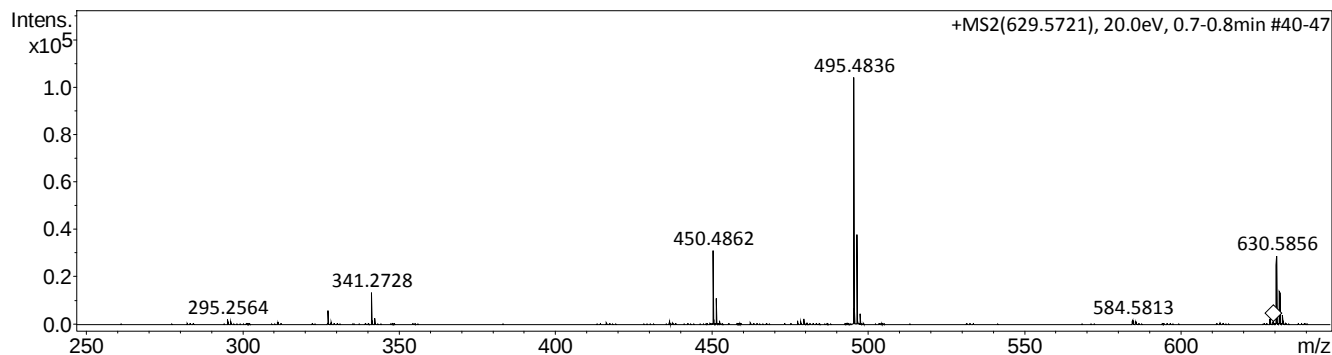

#	m/z	I	I %
1	295.2564	2071	2.0
2	296.2709	1206	1.2
3	311.2534	757	0.7
4	327.2530	5764	5.6
5	328.2554	972	0.9
6	341.2728	13356	12.9
7	342.2747	2495	2.4
8	416.3509	794	0.8
9	436.4684	990	1.0
10	437.4690	425	0.4
11	449.4689	495	0.5
12	450.4862	31083	30.0
13	451.4879	10802	10.4
14	452.4916	1366	1.3
15	462.3568	754	0.7
16	477.4791	1610	1.6
17	478.4869	1182	1.1
18	479.4819	2373	2.3
19	480.4849	679	0.7
20	495.4836	103775	100.0
21	496.4864	37705	36.3
22	497.4906	4540	4.4
23	584.5813	1862	1.8
24	585.5822	981	0.9
25	628.5673	2308	2.2
26	629.5721	1024	1.0
27	630.5856	28649	27.6
28	631.5900	13896	13.4
29	632.5793	3925	3.8
30	633.5748	525	0.5