

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\US-42_P1-D-6_01_5328.d
Method lc_qtof_directospos mrm atorressi.m
Sample Name US-42
Comment Sv: DCM + MeOH + HCOOH
Cecilia Attorresi

Acquisition Date 7/29/2022 9:32:58 AM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

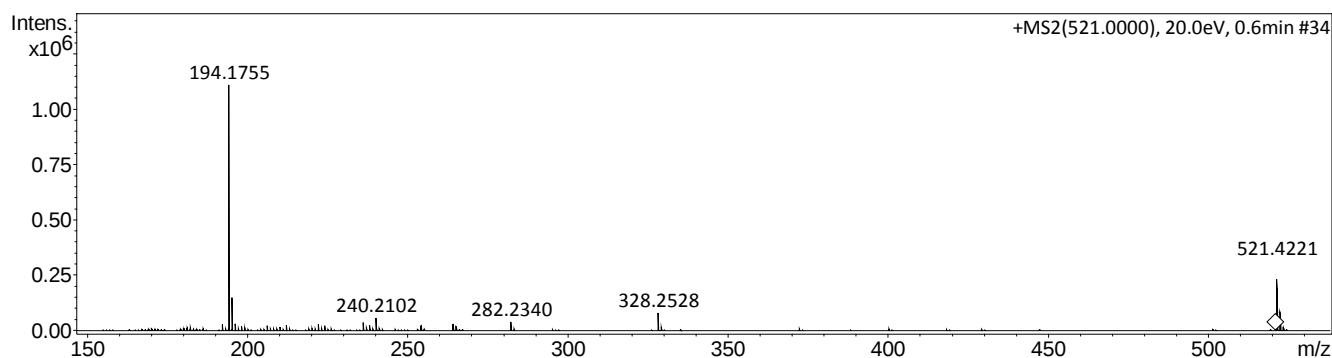

#	m/z	I	I %
1	181.1504	11981	1.1
2	182.1494	12626	1.1
3	192.1584	29356	2.7
4	194.1755	1106851	100.0
5	195.1777	149571	13.5
6	196.1725	30935	2.8
7	197.1721	10150	0.9
8	198.1769	20976	1.9
9	199.1736	13146	1.2
10	206.1748	21645	2.0
11	210.1855	16111	1.5
12	212.2004	26066	2.4
13	220.1773	10496	0.9
14	222.1781	28220	2.5
15	223.1779	10259	0.9
16	224.1746	23047	2.1
17	236.2119	36591	3.3
18	237.2053	13556	1.2
19	238.1951	24058	2.2
20	240.2102	57127	5.2
21	241.2099	11452	1.0
22	254.2274	21880	2.0
23	264.2173	29289	2.6
24	265.2145	18629	1.7
25	282.2340	38948	3.5
26	328.2528	81058	7.3
27	329.2570	16064	1.5
28	521.4221	232251	21.0
29	522.4261	86146	7.8
30	523.4291	12446	1.1