

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\US-44 MRM 556.d
Method Tune_low_format 210120.m
Sample Name US-44 MRM 556
Comment Ceci

Acquisition Date 4/11/2023 10:05:16 AM
Operator ELB
Instrument / Ser# micrOTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	150.0 Vpp	Set Divert Valve	Source

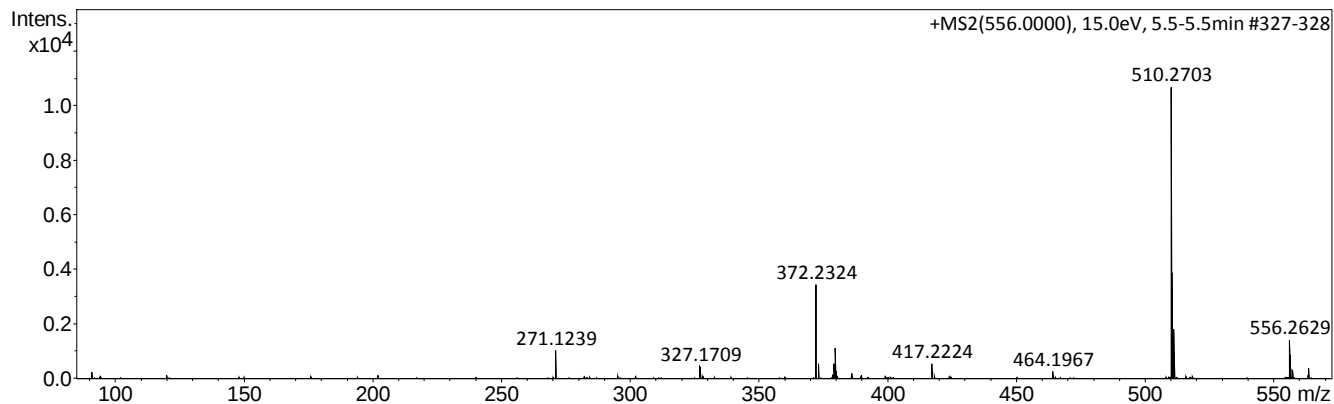

#	m/z	I	I %
1	91.0577	241	2.3
2	120.0813	128	1.2
3	202.0982	116	1.1
4	271.1239	1018	9.5
5	327.1709	450	4.2
6	372.2324	3437	32.2
7	373.2390	529	5.0
8	378.7647	135	1.3
9	379.2995	533	5.0
10	379.4267	410	3.8
11	379.6670	134	1.3
12	379.7814	1123	10.5
13	386.0820	178	1.7
14	389.8991	112	1.1
15	417.2224	536	5.0
16	464.1967	259	2.4
17	510.2703	10659	100.0
18	511.2709	1796	16.8
19	556.2629	1409	13.2
20	557.2654	308	2.9
21	563.5162	247	2.3
22	563.6550	362	3.4