

Qualitative Compound Report

Analysis Info

Analysis Name D:\Data\US44 dias despues_P1-F-3_01_5461.d
Method lc_qtof_directospos.m
Sample Name US44 dias despues
Comment Sv: MeOH + HCOO
Attorressi


Acquisition Date 8/9/2022 3:00:35 p. m.

Operator ELB
Instrument micrOTOF-Q II



Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

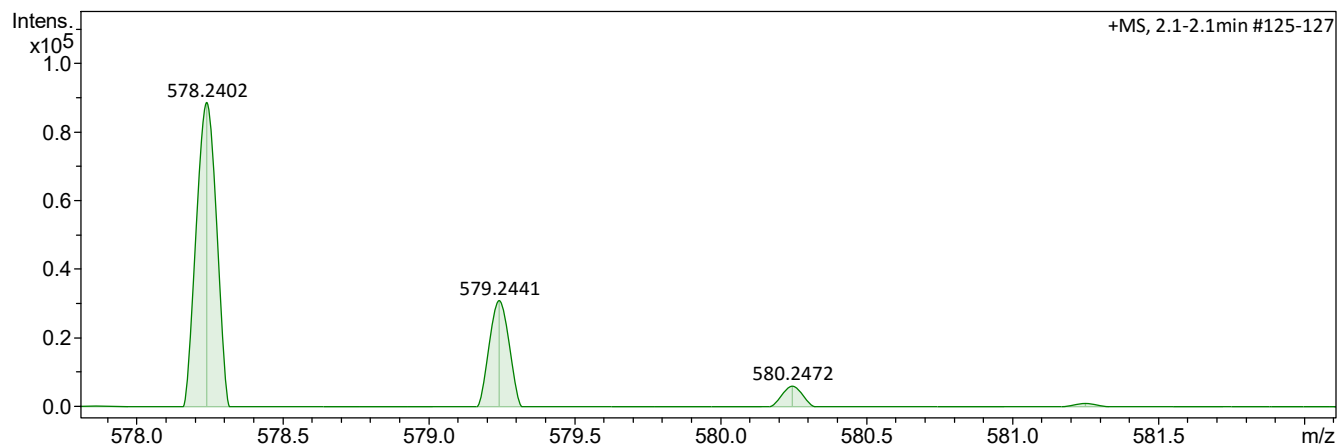

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
578.2402	1	C33H34FN3NaO4	578.2426	4.1	13.0	1	30.67	17.5	even	ok