

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\US-45 ta repeticion_P1-C-3_01_7736.d
Method lc_qtof_directospos mrm atorressi us-45.m
Sample Name US-45 ta repeticion
Comment Sv: MeOH + HCOOH
Cecilia Attoresi

Acquisition Date 8/2/2023 9:31:19 AM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

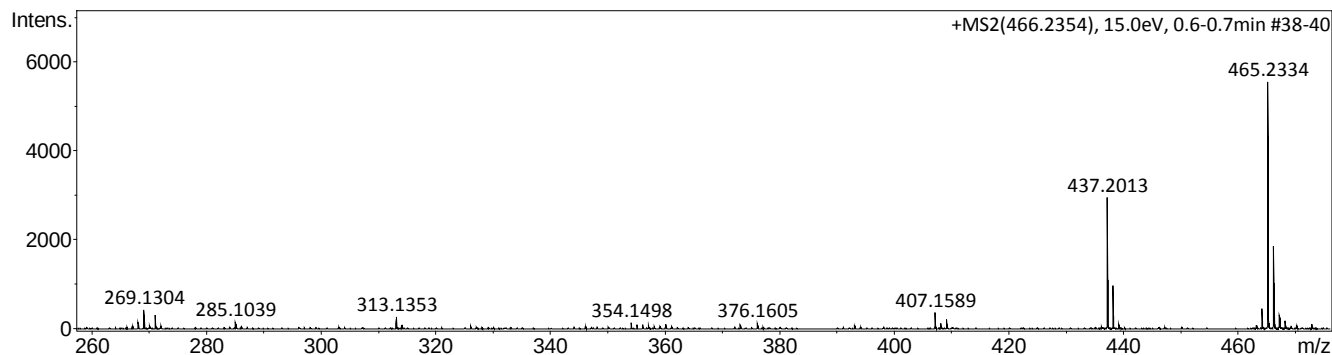

#	m/z	I	I %
1	268.1340	144	2.6
2	269.1304	416	7.5
3	271.1285	302	5.5
4	285.1039	145	2.6
5	313.1353	260	4.7
6	354.1498	132	2.4
7	360.1747	113	2.0
8	376.1605	115	2.1
9	407.1589	361	6.5
10	408.1605	125	2.3
11	409.1788	201	3.6
12	437.2013	2943	53.2
13	438.2050	965	17.4
14	439.2027	109	2.0
15	464.2209	454	8.2
16	465.2334	5536	100.0
17	466.2354	1854	33.5
18	467.2318	308	5.6
19	468.2159	182	3.3
20	472.9133	109	2.0