

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\US-47 crudo de rxn a ta_P1-C-4_01_7733.d
Method lc_qtof_directospos mrm atorressi us-47.m
Sample Name US-47 crudo de rxn a ta
Comment Sv: MeOH + HCOOH
Cecilia Attoresi

Acquisition Date 8/1/2023 2:14:33 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

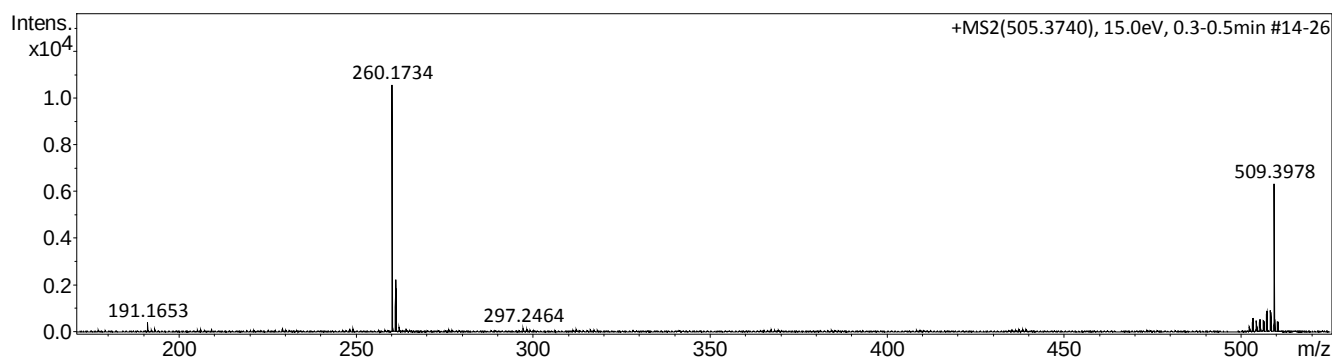

#	m/z	I	I %
1	191.1653	401	3.8
2	193.1795	118	1.1
3	209.1679	124	1.2
4	229.1835	135	1.3
5	248.2237	114	1.1
6	249.1593	135	1.3
7	260.1734	10553	100.0
8	261.1763	2229	21.1
9	262.1875	197	1.9
10	297.2464	141	1.3
11	502.3957	197	1.9
12	503.3767	581	5.5
13	504.3592	474	4.5
14	505.3740	523	5.0
15	506.3916	491	4.7
16	507.3487	855	8.1
17	508.3867	910	8.6
18	509.3978	6325	59.9
19	510.3995	432	4.1