

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\US-47 ta T4-6_P1-C-6_01_7739.d
Method lc_qtof_directospos mrm atorressi us-47 tolueno.m
Sample Name US-47 ta T4-6
Comment Sv: MeOH + HCOOH
Cecilia Attoresi

Acquisition Date 8/2/2023 9:46:46 AM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

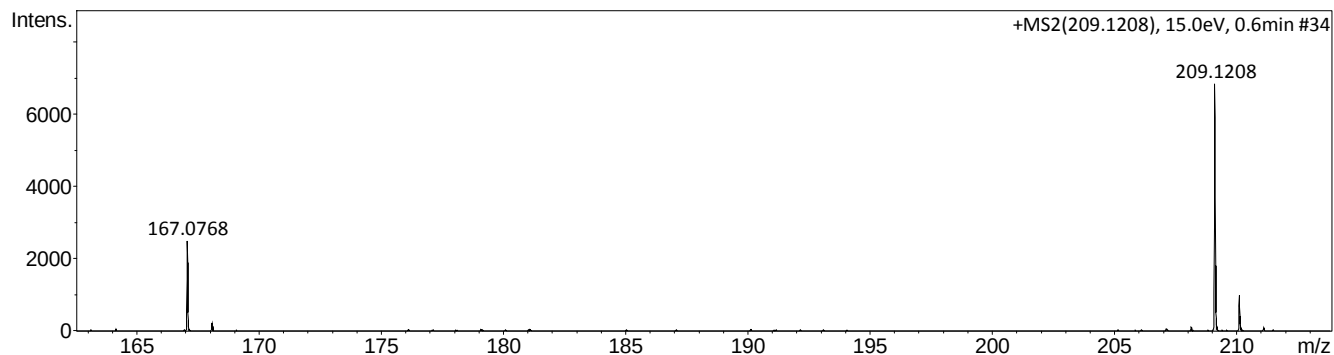

#	m/z	I	I %
1	167.0768	2482	36.4
2	168.0852	214	3.1
3	208.1504	105	1.5
4	209.1208	6816	100.0
5	210.1257	994	14.6