

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\US-47 toluenocrudo de rxn a ta_P1-C-5_01_7738.d
Method lc_qtof_directospos mrm atorressi us-47 tolueno.m
Sample Name US-47 toluenocrudo de rxn a ta
Comment Sv: MeOH + HCOOH
Cecilia Attoresi

Acquisition Date 8/2/2023 9:41:38 AM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

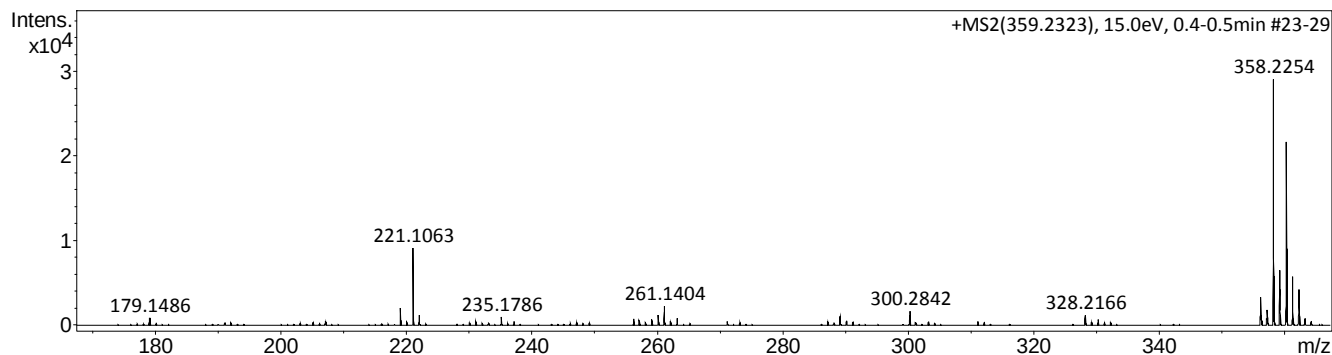

#	m/z	I	I %
1	179.1486	888	3.1
2	219.0925	2069	7.1
3	221.1063	9097	31.4
4	222.1074	1199	4.1
5	231.1252	448	1.5
6	235.1786	1003	3.5
7	237.1931	495	1.7
8	256.2593	748	2.6
9	257.1430	635	2.2
10	259.1568	729	2.5
11	260.1567	1261	4.4
12	261.1404	2254	7.8
13	263.2063	826	2.9
14	271.1541	489	1.7
15	289.1736	1050	3.6
16	290.2016	499	1.7
17	300.2842	1690	5.8
18	303.2248	408	1.4
19	311.1186	513	1.8
20	328.2166	1249	4.3
21	330.2801	671	2.3
22	356.2024	3337	11.5
23	357.2179	1801	6.2
24	358.2254	28968	100.0
25	359.2323	6524	22.5
26	360.2921	21638	74.7
27	361.2938	5741	19.8
28	362.3119	4243	14.6
29	363.2867	772	2.7
30	364.2182	439	1.5