

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\UStol-1_P1-C-2_01_8148.d
Method lc_qtof_directospos mrm atorressi 548.m
Sample Name UStol-1
Comment Sv: DCM + MeOH + HCOOH
Attores

Acquisition Date 10/18/2023 2:28:28 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

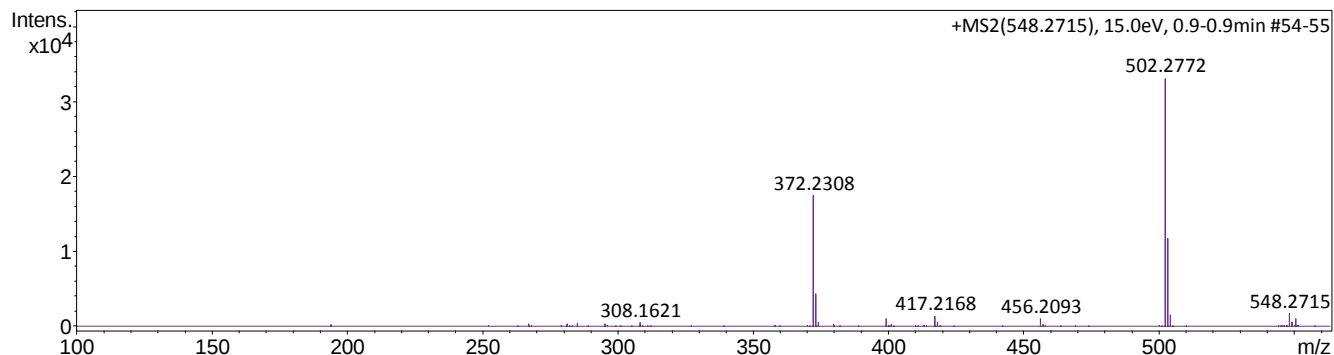

#	m/z	I	I %
1	194.1177	293	0.9
2	267.1492	369	1.1
3	281.1681	327	1.0
4	285.1164	425	1.3
5	295.1760	300	0.9
6	308.1621	504	1.5
7	358.2186	177	0.5
8	372.2308	17427	52.8
9	373.2322	4326	13.1
10	374.2348	489	1.5
11	379.9932	215	0.7
12	399.2146	1021	3.1
13	400.2202	183	0.6
14	401.2266	255	0.8
15	417.2168	1322	4.0
16	418.2161	553	1.7
17	456.2093	1023	3.1
18	457.2145	298	0.9
19	500.2674	183	0.6
20	502.2772	33000	100.0
21	503.2839	11764	35.6
22	504.2837	1507	4.6
23	546.4017	154	0.5
24	547.3488	199	0.6
25	548.2715	1725	5.2
26	549.2811	628	1.9
27	550.2766	200	0.6
28	550.6257	1013	3.1
29	551.2970	213	0.6
30	551.6323	207	0.6