

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\UStol-1_P1-C-2_01_8128.d
Method lc_qtof_directospos.m
Sample Name UStol-1
Comment Sv: DCM + MeOH + HCOOH
Attores

Acquisition Date 10/17/2023 3:39:09 PM
Operator ELB
Instrument / Ser# micrOTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

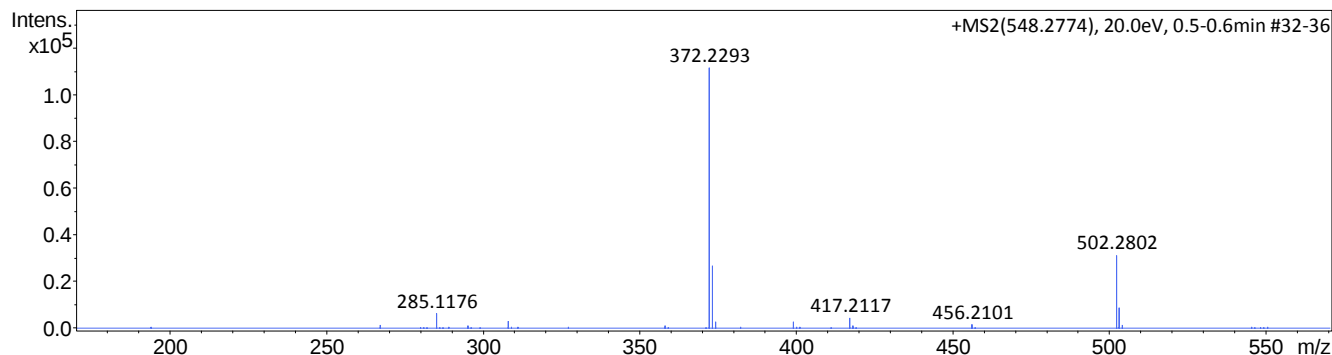

#	m/z	I	I %
1	194.1150	554	0.5
2	267.1443	1517	1.4
3	281.1024	464	0.4
4	285.1176	6371	5.7
5	286.1236	481	0.4
6	289.1265	621	0.6
7	295.1796	1122	1.0
8	308.1606	3174	2.8
9	309.1644	608	0.5
10	311.1720	503	0.5
11	327.1655	528	0.5
12	358.2133	1055	0.9
13	372.2293	111488	100.0
14	373.2324	26751	24.0
15	374.2378	2718	2.4
16	382.1772	764	0.7
17	399.2169	2709	2.4
18	400.2188	766	0.7
19	401.2161	592	0.5
20	417.2117	4425	4.0
21	418.2192	1074	1.0
22	419.2052	404	0.4
23	456.2101	1624	1.5
24	502.2802	31114	27.9
25	503.2811	8872	8.0
26	504.2893	1445	1.3
27	545.4011	645	0.6
28	548.2774	375	0.3
29	549.3018	497	0.4
30	550.6186	545	0.5