

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UStol-2_P1-C-3_01_8149.d
Method lc_qtof_directospos mrm atorressi 707.m
Sample Name UStol-2
Comment Sv: DCM + MeOH + HCOOH
Attores

Acquisition Date 10/18/2023 2:33:34 PM

Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

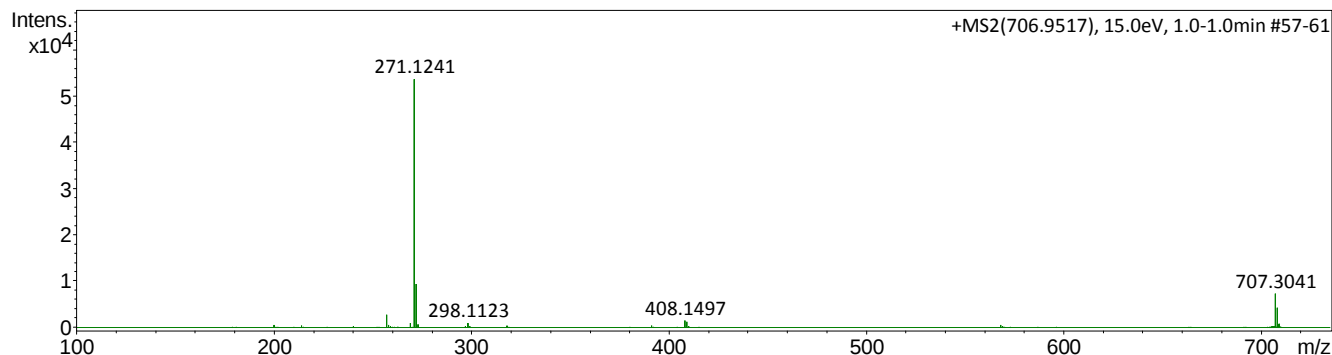

#	m/z	I	I %
1	200.0875	514	1.0
2	214.1034	447	0.8
3	240.0820	185	0.3
4	257.1084	2749	5.1
5	258.1126	532	1.0
6	259.1199	298	0.6
7	269.1083	866	1.6
8	270.1147	168	0.3
9	271.1241	53503	100.0
10	272.1265	9377	17.5
11	273.1277	622	1.2
12	297.1020	184	0.3
13	298.1123	911	1.7
14	299.1186	185	0.3
15	318.1028	416	0.8
16	391.1794	381	0.7
17	408.1497	1457	2.7
18	409.1539	1237	2.3
19	410.1610	305	0.6
20	568.2560	552	1.0
21	569.2557	215	0.4
22	691.4606	149	0.3
23	705.4964	199	0.4
24	706.4781	231	0.4
25	707.3041	7255	13.6
26	708.3015	4227	7.9
27	708.4510	599	1.1
28	708.9582	222	0.4
29	709.3131	747	1.4
30	709.4569	181	0.3