

Qualitative Compound Report

Analysis Info

Analysis Name D:\Data\ggc\UStol-2_P1-C-3_01_8129.d
Method lc_qtof_directospos.m
Sample Name UStol-2
Comment Sv: DCM + MeOH + HCOOH
Attoresi


Acquisition Date 10/17/2023 3:44:20 PM

Operator ELB
Instrument micrOTOF-Q II



Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

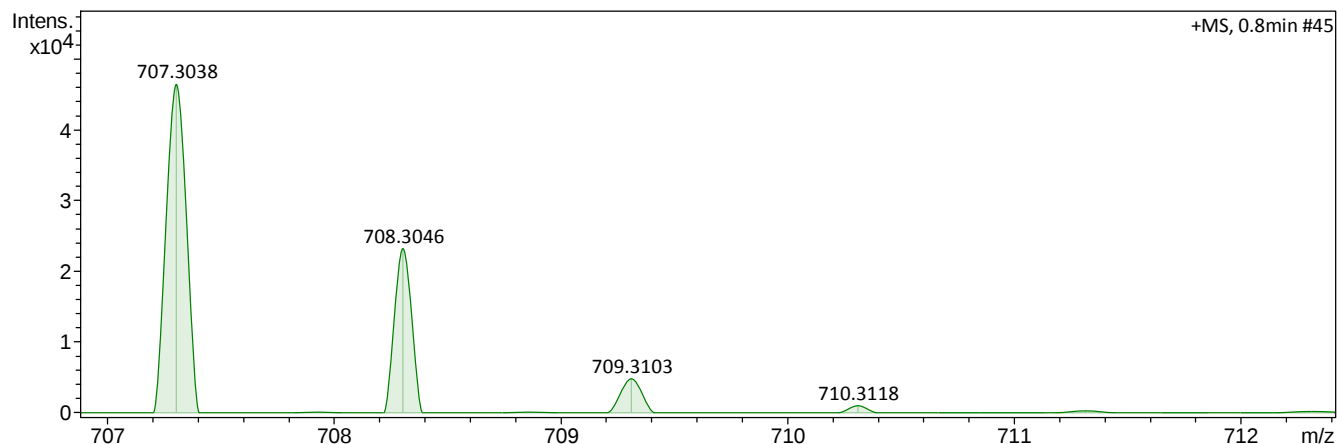

Meas. m/z	#	Ion Formula	m/z	err [ppm]	mSigma	# mSigma	Score	rdb	e ⁻ Conf	N-Rule
707.3038	1	C ₄₁ H ₄₁ F ₂ N ₄ O ₅	707.3040	0.2	18.8	2	100.00	22.5	even	ok