

Mass Spectrum List Report

Analysis Info


Analysis Name D:\Data\ggc\UStol-3_P1-C-4_01_8153.d
Method lc_qtof_directospos mrm atorressi 657.m
Sample Name UStol-3
Comment Sv: DCM + MeOH + HCOOH
Attores

Acquisition Date 10/18/2023 3:11:18 PM

Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	100 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1500 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

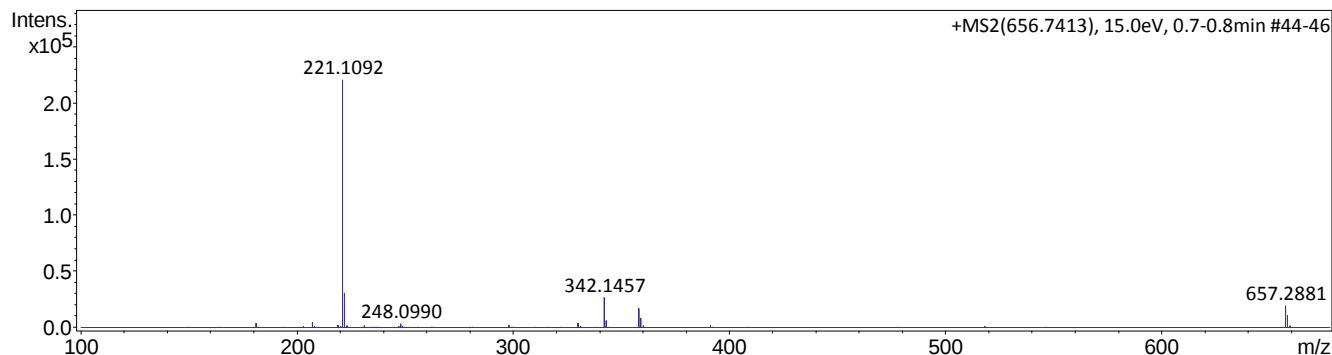

#	m/z	I	I %
1	181.0763	3618	1.6
2	182.0790	533	0.2
3	203.0962	790	0.4
4	207.0916	4616	2.1
5	208.0972	731	0.3
6	209.1063	502	0.2
7	219.0921	2103	1.0
8	220.1006	1154	0.5
9	221.1092	220181	100.0
10	222.1117	30695	13.9
11	223.1146	1762	0.8
12	231.0926	1340	0.6
13	247.0892	872	0.4
14	248.0990	3445	1.6
15	249.1006	741	0.3
16	298.1474	1915	0.9
17	330.1081	3559	1.6
18	331.1132	728	0.3
19	338.1782	505	0.2
20	342.1457	26818	12.2
21	343.1475	6047	2.7
22	358.1397	16934	7.7
23	359.1452	8519	3.9
24	360.1493	1649	0.7
25	391.1847	1852	0.8
26	392.1877	528	0.2
27	518.2534	1163	0.5
28	657.2881	19306	8.8
29	658.2945	10826	4.9
30	659.2980	1509	0.7