

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\UStol-3_P1-C-4_01_8130.d
Method lc_qtof_directospos.m
Sample Name UStol-3
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 3:49:32 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

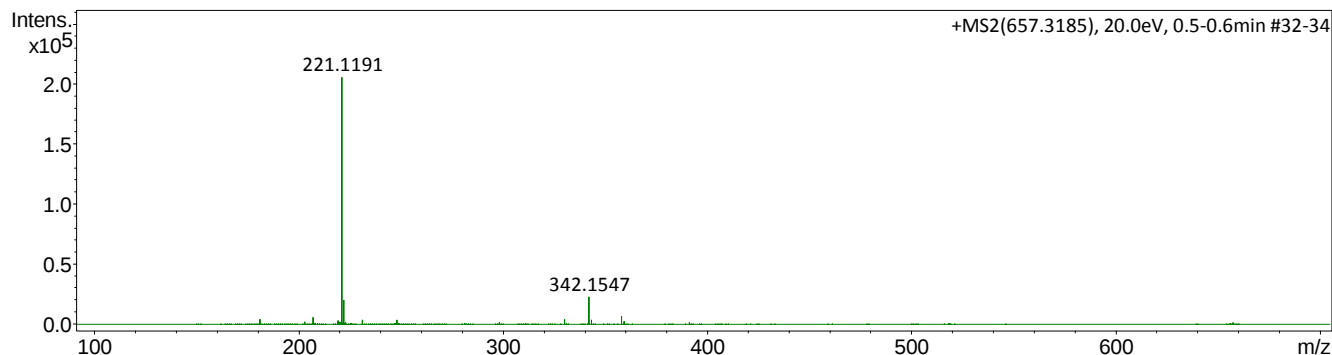

#	m/z	I	I %
1	181.0856	3791	1.8
2	203.1071	1810	0.9
3	205.0865	439	0.2
4	207.1029	5678	2.8
5	208.1054	624	0.3
6	209.1150	572	0.3
7	219.1018	2770	1.3
8	220.1098	1720	0.8
9	221.1191	205488	100.0
10	222.1215	19854	9.7
11	223.1229	1209	0.6
12	231.1029	3449	1.7
13	232.1054	411	0.2
14	236.1177	505	0.2
15	247.1007	604	0.3
16	248.1057	3347	1.6
17	249.1121	601	0.3
18	280.1496	533	0.3
19	281.1528	647	0.3
20	298.1548	1584	0.8
21	330.1198	4136	2.0
22	331.1246	594	0.3
23	342.1547	22339	10.9
24	343.1587	3406	1.7
25	358.1504	6462	3.1
26	359.1586	2571	1.3
27	391.1981	1120	0.5
28	518.2631	748	0.4
29	657.3185	1557	0.8
30	658.3133	507	0.2