

Mass Spectrum List Report


Analysis Info

Analysis Name D:\Data\ggc\UStol-4_P1-C-5_01_8131.d
Method lc_qtof_directospos.m
Sample Name UStol-4
Comment Sv: DCM + MeOH + HCOOH
Attoresi

Acquisition Date 10/17/2023 3:54:42 PM
Operator ELB
Instrument / Ser# microTOF-Q II 228888.10
193

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	3.5 Bar
Focus	Not active	Set Capillary	4000 V	Set Dry Heater	200 °C
Scan Begin	70 m/z	Set End Plate Offset	-500 V	Set Dry Gas	7.0 l/min
Scan End	1000 m/z	Set Collision Cell RF	300.0 Vpp	Set Divert Valve	Source

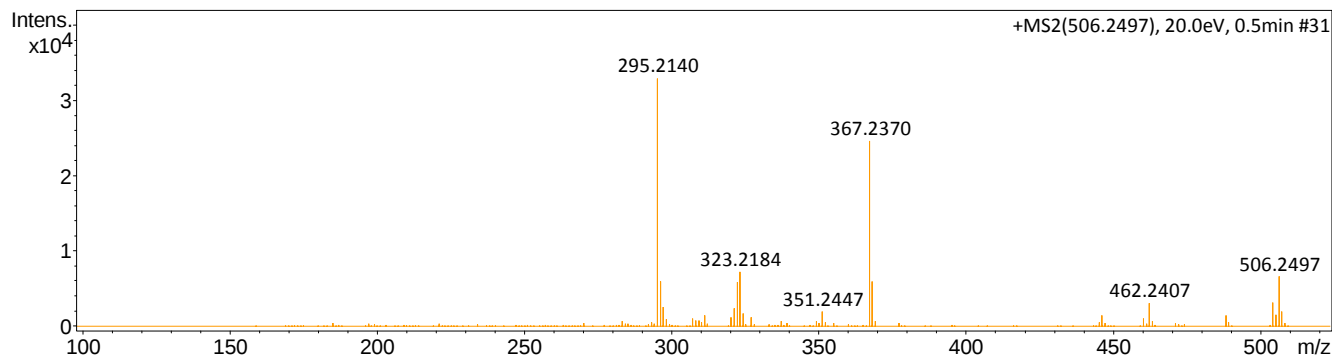

#	m/z	I	I %
1	283.2089	640	1.9
2	295.2140	32829	100.0
3	296.2175	5931	18.1
4	297.2291	2556	7.8
5	298.2222	953	2.9
6	307.2151	980	3.0
7	308.2304	805	2.5
8	309.2324	783	2.4
9	311.2128	1428	4.3
10	320.2286	1200	3.7
11	321.2269	2382	7.3
12	322.2518	5837	17.8
13	323.2184	7175	21.9
14	324.2192	1712	5.2
15	327.2085	1180	3.6
16	337.2274	684	2.1
17	349.2273	653	2.0
18	351.2447	1924	5.9
19	367.2370	24565	74.8
20	368.2420	5887	17.9
21	369.2466	638	1.9
22	446.2480	1450	4.4
23	460.2643	1059	3.2
24	462.2407	3064	9.3
25	463.2444	717	2.2
26	488.2479	1470	4.5
27	504.2378	3174	9.7
28	505.2432	1543	4.7
29	506.2497	6612	20.1
30	507.2656	1937	5.9